



**STARTER 3100M  
Multi-parameter Bench Meter  
Instruction Manual**

## TABLE OF CONTENTS

<b>1</b>	<b>INTRODUCTION .....</b>	<b>1</b>
1.1	Definition of Signal Warnings and Symbols .....	1
1.2	Safety Precautions .....	2
1.3	Display and controls .....	3
<b>2</b>	<b>INSTALLATION .....</b>	<b>5</b>
2.1	Package contents .....	5
2.2	Installing the stand-alone electrode holder .....	6
2.3	Installing the power adapter .....	7
2.4	Connect the electrodes .....	7
2.5	Meter stand for adjusting view angle .....	8
2.6	Attached quick guide .....	8
<b>3</b>	<b>ST3100M pH Operation .....</b>	<b>9</b>
3.1	Setup .....	9
3.1.1	Set temperature unit and MTC value .....	9
3.1.2	Selecting a predefined buffer group .....	10
3.2	Calibration .....	11
3.2.1	Performing 1-point calibration .....	11
3.2.2	Performing 2-point calibration .....	12
3.3	Sample Measurement .....	13
3.3.1	pH measurement .....	13
3.3.2	mV measurement .....	13
<b>4</b>	<b>ST3100M Conductivity Operation .....</b>	<b>13</b>
4.1	Setup .....	13
4.1.1	Set temperature unit .....	13
4.1.2	Set MTC temperature value .....	13
4.1.3	Set calibration standard point .....	14
4.1.4	Set temperature correction coefficient .....	14
4.1.5	Set TDS factor .....	14
4.2	Calibration .....	14
4.2.1	Selecting a standard .....	15
4.2.2	Performing a calibration .....	15
4.3	Sample measurement .....	16
4.3.1	Conductivity measurement .....	16
4.3.2	TDS, Salinity or Resistivity measurement .....	16
<b>5</b>	<b>Using the memory .....</b>	<b>17</b>
5.1	Storing a reading .....	17
5.2	Recalling from memory .....	17
5.3	Clearing the memory .....	17
<b>6</b>	<b>Printing .....</b>	<b>17</b>

<b>7</b>	<b>MAINTENANCE .....</b>	<b>20</b>
7.1	Error message.....	20
7.2	Meter maintenance.....	21
7.3	Self-diagnosis.....	21
7.4	Recover factory settings.....	21
<b>8</b>	<b>TECHNICAL DATA.....</b>	<b>22</b>
8.1	Specifications .....	22
8.2	Compliance .....	23
<b>9</b>	<b>Appendix .....</b>	<b>24</b>
9.1	pH Buffer Groups .....	24
9.2	Conductivity standards.....	25
9.3	Examples of temperature coefficients ( $\alpha$ -value).....	26
9.4	Conductivity to TDS conversion factors .....	26

## 1 INTRODUCTION

Thank you for choosing OHAUS!

Please read the manual completely before using the STARTER 3100M multi-parameter bench meter to ensure proper setup, operation and maintenance. STARTER 3100M multi-parameter bench meter can measure pH, ORP; Temperature; Conductivity/TDS/Resistivity/Salinity values.

STARTER 3100M multi-parameter bench meter has an excellent performance/price ratio and is designed with many useful features including a stand-alone electrode holder and a beeper for error alert. Other accessories such as pH electrodes and buffer solutions are also available.

STARTER 3100M multi-parameter bench meter offers many practical features and functions such as:

- Large backlit LCD with Quick Guide attached under the meter to assist with user operation
- Stand-alone electrode holder for maximum flexibility
- Electrode condition icon automatically showing you the health of your pH electrode
- memory to store up to 99 pH measurements and 99 conductivity measurements

### 1.1 Definition of Signal Warnings and Symbols

Safety notes are marked with signal words and warning symbols. These show safety issues and warnings. Ignoring the safety notes may lead to personal injury, damage to the instrument, malfunctions and false results.

#### Signal Words

<b>WARNING</b>	For a hazardous situation with medium risk, possibly resulting in injuries or death if not avoided.
<b>CAUTION</b>	For a hazardous situation with low risk, resulting in damage to the device or the property or in loss of data, or injuries if not avoided.
<b>Attention</b>	For important information about the product.
<b>Note</b>	For useful information about the product

#### Warning Symbols



General hazard



Explosion hazard



Corrosive hazard



Alternating current



Direct current


## 1.2 Safety Precautions

**CAUTION:** Read all safety warnings before installing, making connections, or servicing this equipment. Failure to comply with these warnings could result in personal injury and/or property damage. Retain all instructions for future reference.

- Verify that the input voltage range printed on the data label and the plug type matches the local AC power to be used.
- Make sure that the power cord does not pose a potential obstacle or tripping hazard.
- Use the equipment only in dry locations.
- Dry off any liquid spills immediately. The instrument is not watertight.
- When using chemicals and solvents, comply with the instructions of the chemical producer and the general lab safety rules.
- Use only approved accessories and peripherals.
- Operate the equipment only under ambient conditions specified in these instructions.
- Disconnect the equipment from the power supply when cleaning.
- Do not operate the equipment in hazardous or unstable environments.
- Service should only be performed by authorized personnel.





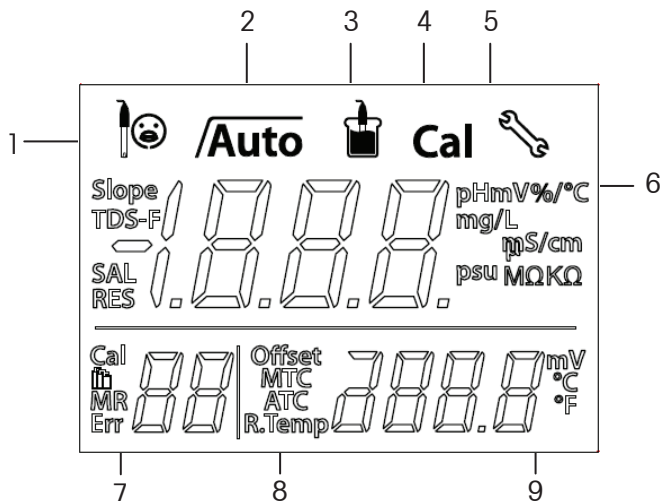








1.3 Display and controls

Displays



- 1 pH Electrode condition
  - ☺ Slope: more than 95% and offset: ± (0-15) mV  
Electrode condition is good
  - ☺ Slope: 90-95% or offset: ± (15-35) mV  
Electrode condition is acceptable
  - ☹ Slope: less than 90% or offset: ± (35-60) mV  
Electrode condition is not good or needs cleaning
- 2 Endpoint stability icon ; Auto endpoint icon **Auto**.
- 3 Measurement icon - ; means measurement or calibration is running when blinks.
- 4 Calibration icon - **Cal**; means calibration in progress when display.
- 5 Setup icon - ; instrument is in the setup mode, can set temperature(MTC), buffer group etc.
- 6 pH/mV reading, or slope of pH electrode calibration; or Conductivity/TDS/Salinity/Resistivity value, or cell constant of conductivity electrode.
- 7 Calibration point **Cal** / Buffer group /Memory number **MR**/ Error index **Err**.
- 8 Auto temperature compensation - **ATC** ; Manual temperature compensation – **MTC**; Conductivity reference temperature - **R.Temp**
- 9 Temperature value during measurement or offset (mV) value in pH calibration process.

Controls

Button	Press & release 	Press & hold for 3 seconds 
	- Switch between pH(mV) parameter and conductivity(TDS/Salinity/Resistivity) parameter when at measurement interface	
	- Start or finish measurement - Confirm setting, store entered value	- Turn auto endpoint on / off 
	- Start calibration	- Recall the latest calibration data : slope and offset
	- Meter turn on - Exit and return to measurement screen	- Meter turn off
	- Store current reading to memory - Increase value during setting - Scroll up through the memory	- Recall stored data - Print current memory data
	- Switch between pH and mV - Switch between conductivity, TDS, Salinity and Resistivity - Decrease value during setting - Scroll down through the memory	- Enter setup mode
 	- Start self-diagnosis	
 		Turn on/turn off the backlight of the LCD

## 2 INSTALLATION

Carefully unpack the box.

### 2.1 Package contents

The model ST3100M-B multi-parameter bench meter (basic package) has the following items:

ST3100M-B	Units
STARTER 3100M	1
Stand-alone electrode holder (include holder base, screw and arm)	1 set
In use cover	1
1413 $\mu\text{S}/\text{cm}$ standard solution	1 bottle (about 20ml)
12.88 $\text{mS}/\text{cm}$ standard solution	1 bottle (about 20ml)
12V Power supply	1 set
RS232 Interface, Scout (Mini-din to RS232 cable)	1

In addition to ST3100M-B multi-parameter bench meter content, the ST3100M-F multi-parameter bench meter package also includes the following:

pH Buffer Powder Set (4.01, 7.00, 10.01)	1 set
ST310 3-in-1 refillable pH electrode	1
STCON3 4-ring conductivity electrode	1

Each pH buffer powder should be dissolved in 250ml pure water or deionized water in a volumetric flask.

The best measurement range for STCON3 4-ring (or 4-pole) conductivity electrode is  $70\mu\text{S}/\text{cm}$ - $200\text{mS}/\text{cm}$ . In this range the measurement accuracy can reach 0.5%.

If you use STCON3 to measure pure water which conductivity value is below  $70\mu\text{S}/\text{cm}$ ; the measurement will be less accurate (approximately 1% to 5%).

Do not use STCON3 to measure conductivity value less than  $2\mu\text{S}/\text{cm}$ , the accuracy is not good.

We have STCON7 pure water conductivity electrode which measurement range is  $0.02\mu\text{S}/\text{cm}$ - $200\mu\text{S}/\text{cm}$ , with accuracy of  $0.02\mu\text{S}/\text{cm}$ .


Additional electrodes available include the followings:

Model	Description
STCON3	4-ring conductivity electrode ( $70\mu\text{S}/\text{cm}$ - $200\text{mS}/\text{cm}$ .)
STCON7	Pure water 2-pole conductivity electrode ( $0.02\mu\text{S}/\text{cm}$ - $200\mu\text{S}/\text{cm}$ )
ST310	3-in-1 plastic refillable pH electrode


ST320	3-in-1 plastic gel pH electrode(no need to fill)
ST350	3-in-1 glass refillable pH electrode
ST210	2-in-1 plastic refillable pH electrode
ST230	2-in 1 glass muddy sample pH electrode
ST260	2-in 1 glass tris-buffer pH electrode
ST270	2-in 1 glass pierce pH electrode
STORP1	Gel plastic ORP electrode
STORP2	Refillable glass ORP electrode
STTEMP30	Temperature Electrode

## 2.2 Installing the stand-alone electrode holder

Install the electrode arm on the base,

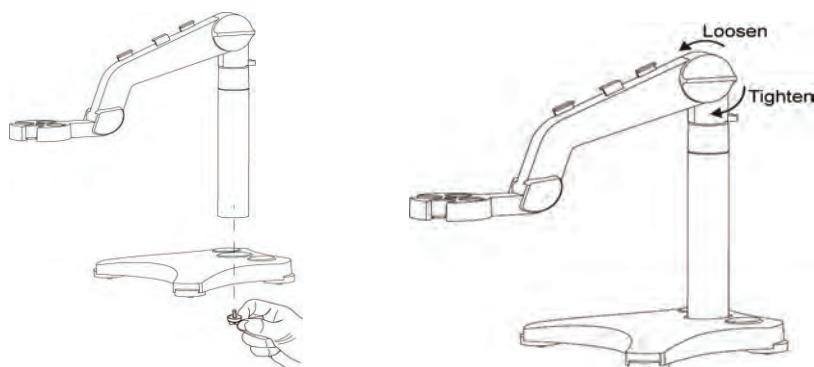


After adjusting the tension knob to some extent, you can move the upper arm up and down. When the pH electrode is installed on the arm, the storage bottle of pH electrode fits into the base hole.

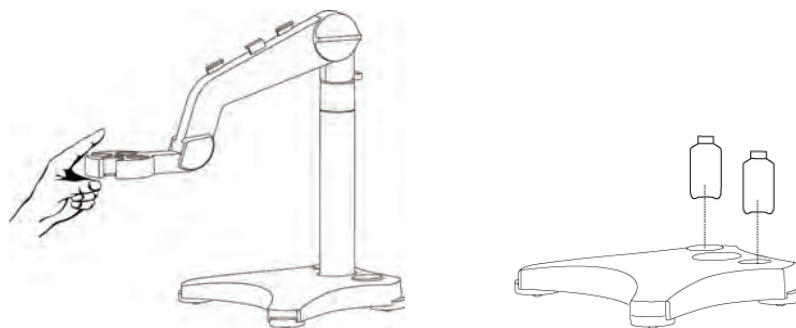

### 2.3 Installing the power adapter

Insert the right adapter clip into the power adapter slot. The Ohaus balance power supply is also 12V which could also be used for the pH meter.

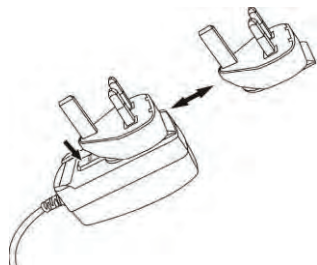

### 2.4 Connect the electrodes


There are several sockets for ST3100M.


"BNC" socket for pH electrode,

"TEMP." Socket (Cinch) for temperature electrode,

"Min-Din" Socket for conductivity electrode,

"Data" socket can connect printer through a connect cable (RS232 Interface, Scout ; from the mini-din to RS232, item NO 30268982) which is included in the kits.

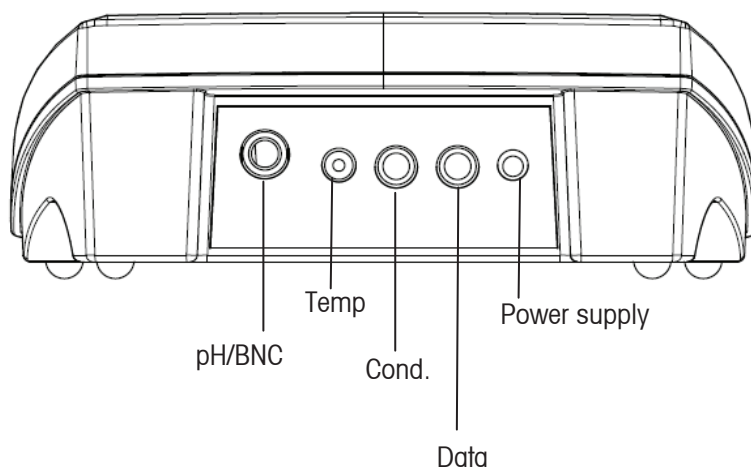

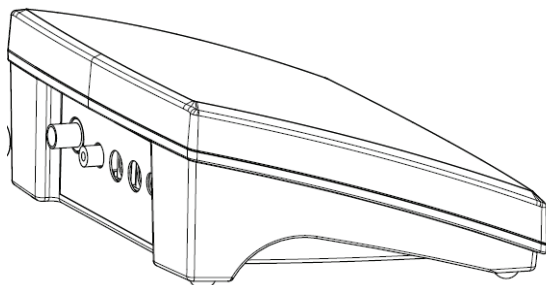

For ST310 electrode connect to the BNC and Cinch socket. For 2-in-1 pH electrode (e.g. ST210) you only need to connect to the BNC. Temp. socket is for a separate temperature electrode.

STCON3 or STCON7 have a built-in temperature sensor which do not need a separate temperature electrode.

### **2.5 Meter stand for adjusting viewing angle**

One unique design feature of the STARTER 3100M is the meter stand, which can be used to adjust the viewing angle of the display in case of working on a high table.

### **2.6 Attached quick guide**

Another unique design feature of the STARTER 3100M is the attached quick guide, the quick guide is attached into the bottom housing of the meter.

### 3 ST3100M pH Operation



**WARNING** Do not operate the equipment in hazardous environments. The equipment is not explosion protected.



**WARNING** When using chemicals and solvents, comply with the instructions of the chemical producer and the general lab safety rules.







#### 3.1 Setup

##### 3.1.1 Set temperature unit and MTC value





Please note:

If a temperature electrode is used, Automatic Temperature Compensation (**ATC**) and the sample temperature are displayed on the screen. You may then choose to skip MTC setup (below). If the meter does not detect a temperature electrode or one is not used, the meter automatically switches to Manual Temperature Compensation (**MTC**) mode and **MTC** appears on the screen.

MTC can be set as follows:

- Power on the meter by pressing .
- Press and hold  until the setup icon  appears on the display and the current temperature unit blinks ( $^{\circ}\text{C}$  or  $^{\circ}\text{F}$ ).
- Press  or  to switch between  $^{\circ}\text{C}$  and  $^{\circ}\text{F}$ .
- Press  to confirm your selection.

Then

- ❖ Continue with MTC temperature setting by using  or  to adjust temperature compensation accordingly
- ❖ Press  to confirm the setting
- ❖ Press  to return to the measurement screen.

The default MTC temperature value setting is  $25^{\circ}\text{C}$  ( $77^{\circ}\text{F}$ ).

**Note:**  $^{\circ}\text{C} = 5/9 (^{\circ}\text{F} - 32)$

**Note:** STARTER 3100M accepts **NTC 30 k $\Omega$**  temperature sensor.

### 3.1.2 Selecting a predefined buffer group

After confirming the MTC compensation temperature value, make the buffer group selection. Use



or



to select a buffer group among 6 buffer groups. Press



to confirm the setting or press to leave to return to the measurement screen.

The default buffer group is **b1**.

<b>b1</b>	1.68	4.01	7.00	10.01
-----------	------	------	------	-------

Please note:

There are 6 buffer groups in the meter, you can select the buffer group you prefer, the buffer value will be automatically recognized during calibration. The 6 predefined buffer groups are (at 25°C):

<b>b1 (US)</b>	<b>1.68</b>	<b>4.01</b>	<b>7.00</b>	<b>10.01</b>	
<b>b2 (EU)</b>	2.00	4.01	7.00	9.21	11.00
<b>b3 (MERCK)</b>	2.00	4.00	7.00	9.00	12.00
<b>b4 (DIN)</b>	1.09	4.65	6.79	9.23	12.75
<b>b5 (JJG)</b>	1.68	4.00	6.86	9.18	12.46
<b>b6 (JIS Z)</b>	1.68	4.01	6.86	9.18	

ST3100M automatically corrects for the temperature dependence of the buffer pH values given in the following table - buffer group **b1**.

This means, if the buffer solutions' temperature is 15°C, the calibration value you will get should be pH1.67 (buffer 1.68), pH4.00 (buffer 4.01), pH7.04 (buffer 7.00) and pH10.12 (buffer 10.01).

5 °C	1.67	4.01	7.09	10.25
10 °C	1.67	4.00	7.06	10.18
<b>15 °C</b>	<b>1.67</b>	<b>4.00</b>	<b>7.04</b>	<b>10.12</b>
20 °C	1.68	4.00	7.02	10.06
<b>25 °C</b>	<b>1.68</b>	<b>4.01</b>	<b>7.00</b>	<b>10.01</b>
30 °C	1.68	4.01	6.99	9.97
35 °C	1.69	4.02	6.98	9.93
40 °C	1.69	4.03	6.97	9.89
45 °C	1.70	4.05	6.97	9.86
50 °C	1.71	4.06	6.96	9.83

### 3.2 Calibration

Standard procedure of pH measurement is as follows:

- pH electrode preparation
- buffer preparation and pH electrode calibration
- sample preparation
- pH measurement
- Record measurement results or print
- Rinse the pH electrode and properly store

pH electrode preparation: pH electrode should be rinsed with pure water before and after use. Check if the electrode is physically damaged. (Be careful with the glass bulb)

Note: please calibrate the pH electrode before measurement.

STARTER 3100M can perform 1-, 2- or 3- point calibrations.

**Calibration:** pH electrodes need to be calibrated with pH standard buffer solution before a proper pH measurement can be made. **Calibration** is to display the correct pH value when meter receive the mV value signal from the pH electrode.




Slope: the linear coefficient between mV and pH according to theoretical value (e.g. - 59.16mV/pH @ 25°C which means 100% slope);

Offset: the mV value when pH value is 7.00. (Theoretical value is 0 mV);

#### 3.2.1 Performing 1-point calibration




When performing calibration, Ohaus recommends using **Auto End Point Mode**. After powering the meter on, be sure the top of the screen shows  $\sqrt{\text{Auto}}$  to ensure the meter is in **Auto End point Mode**.

**Auto or Manual End point Mode:**




- Press and hold  to change the **End Point Mode**.
- When in Manual Mode, to manually reach a pH measurement or calibration value, you need to press button-  when reading is stable and displays  $\sqrt{\quad}$ : then the sample reading or calibration value freezes,  $\sqrt{\quad}$  blinks 3 times and freezes on the display.
- When in Auto End Point Mode, the meter determines when the reading is stable then displays and locks the reading or calibration value automatically, the reading freezes and  blinks 3 times then disappears;  $\sqrt{\text{Auto}}$  blinks 3 times and freezes on the display.

**Note:** With the 1-point calibration only the **offset** is adjusted. If the sensor was previously calibrated with multi-point calibration the previously stored **slope** will remain. Otherwise theoretical **100% slope** (-59.16 mV / pH) will be used.




When STARTER 3100M is in **pH measurement mode**; place the pH electrode in a calibration buffer, stir 5 seconds, wait for 30 seconds, then:

- Press  "Cal 1" displays on the bottom left of the screen and "Cal" is blinking. Cal and  appear on the top of the screen,  is blinking during calibration.
- The meter reaches **endpoint** automatically according to the **preselected auto-endpoint mode**, the calibration point pH value (e.g. 7.00) with the temperature display on the screen.




The 1-point calibration is finished; There are now 3 options (OHAUS recommends conducting at least a 2 point calibration);

- Press  to do the 2-point calibration.
- Press  to store the 1-point calibration and exit, the **offset** and the **slope** are shown on the display for 3 seconds then return to the measurement screen.
- Press  to reject the calibration, return to the measurement screen.

### 3.2.2 Performing 2-point calibration

- Perform 1-point calibration as described above.
- Rinse the pH electrode with pure water and wipe off with tissue.
- Place the electrode in the next calibration buffer, stir and wait, then press , "Cal 2" displays on the bottom left of the screen and "Cal" is blinking. On the top of the screen Cal and  appear,  is blinking during calibration.
- The meter reaches endpoint according to the endpoint mode, the calibration point pH value (e.g. 4.01) with the temperature display on the screen.




The 2-point calibration is finished. There are 3 options:

- Press  to do the 3-point calibration.
- Press  to store the 2-point calibration and exit, the **offset** and **slope** are shown on the display for 3 seconds then return to the measurement screen.
- Press  to reject the calibration, return to the measurement screen.


**Note:** To perform a 3 point calibration, follow the instructions for performing a 2 point calibration using a third buffer.

### 3.3 Sample Measurement



#### 3.3.1 pH measurement

- Place the pH electrode in the sample. Stir for 5 seconds; wait for 30 seconds.
- Press  to start the pH measurement,  appears on the display.  is blinking during measurement.
- When meter reaches endpoint, the pH value with the temperature display on the screen.

#### 3.3.2 mV measurement







- Press  to switch between **pH measurement mode** and **mV measurement mode**.
- Follow the same procedure as for pH measurement to perform mV measurement.

## 4 ST3100M Conductivity Operation

After turning on the meter by pressing , press  to switch from pH parameter to conductivity parameter.

### 4.1 Setup



#### 4.1.1 Set temperature unit



- Press and hold  until the set up icon  appears on the display and the current temperature unit blinks. (°C or °F)
- Use  or  buttons to select temperature unit .
- Press  to confirm your setting. Continue with temperature value setting by following or press  to go back to the measurement screen.

Note: °C = 5/9 (°F -32)

#### 4.1.2 Set MTC temperature value

After the temperature unit setting, the meter goes to setup manual temperature (MTC) value setting.



Use  or  buttons to adjust the temperature value.



Press  to confirm your setting. Continue with calibration standard setting by following or press  to go back to the measurement screen.

#### 4.1.3 Set calibration standard point

After the MTC temperature value setting, the meter goes to setup calibration standard. The 5 predefined standard points are:

10 $\mu\text{S/cm}$	84 $\mu\text{S/cm}$	500 $\mu\text{S/cm}$	1413 $\mu\text{S/cm}$	12.88 mS/cm
---------------------	---------------------	----------------------	-----------------------	-------------



Use the  or  buttons to select calibration standard.

Press  to confirm your setting. Continue with temperature correction coefficient setting by following the steps in 4.1.4 or press  to go back to the measurement screen.

#### 4.1.4 Set temperature correction coefficient

After the calibration standard setting, the meter goes to the temperature correction coefficient setting.

Use the  or  buttons to adjust the temperature correction value. (0.00 to 10.00  $\%/^{\circ}\text{C}$ ).





Press  to confirm your setting. Continue with reference temperature setting by following the steps or press  to go back to the measurement screen.

#### Note:

If you set the temperature correction coefficient value as 0  $\%/^{\circ}\text{C}$ , that means **no Temperature Compensation** for the conductivity measurement. The meter displays the real conductivity value at current temperature without compensation.

#### 4.1.5 Set TDS factor

After selecting the reference temperature, the current TDS factor blinks.







Use  or  buttons to adjust the TDS factor value. Press  to confirm your setting or press  to go back to the measurement screen.

### 4.2 Calibration

The first time you use the conductivity electrode, it should be calibrated before taking any measurement. Please also read the conductivity electrode instruction manual for reference.

#### 4.2.1 Selecting a standard

When using the STARTER 3100M conductivity meter, you have to select a standard for calibration (see 3.3).


Press and hold the  enter setup mode, after press  to confirm the temperature unit and value. Then the current standard blinks. Use  or  buttons to select the standards, press  to confirm. Press  to leave the setup mode.

The 5 predefined standards are:


10 $\mu\text{S}/\text{cm}$	84 $\mu\text{S}/\text{cm}$	500 $\mu\text{S}/\text{cm}$	1413 $\mu\text{S}/\text{cm}$	12.88 $\text{mS}/\text{cm}$
----------------------------	----------------------------	-----------------------------	------------------------------	-----------------------------



Tables for automatic temperature compensation are programmed in the meter for each standard (see appendix).


#### 4.2.2 Performing a calibration


When performing calibration, Ohaus recommends using **Auto End Point Mode**. After powering the meter on, be sure the top of the screen shows  to ensure the meter is in **Auto End point Mode**.

About Auto or Manual End point Mode, please see 3.2.1.

Place the conductivity electrode in the selected calibration standard solution, wait 10-15s, then press .

The calibration icon **Cal** and the measurement icon  appear on the display. The icon  is blinking during calibration measurement. The meter reaches endpoint automatically according to the preselected auto-endpoint mode after the signal has stabilized.

When the calibration is finished, the standard value is displayed and stored; the measurement icon  blinks 3 times and disappears.



To finish the calibration and return to the sample measurement, press . The cal. data--cell constant is then shown on the display for 3 seconds.

**Note:**

To ensure the most accurate conductivity readings, you should verify your cell constant with a standard solution before measurement and recalibrate if necessary. Always use fresh standards. For STCON3 the normal cell constant range is 1.50 – 2.00. (e.g. 1.71 /cm) if the cell constant is outside the range due to an improper calibration, you may need to recover factory settings (see 5.4), then repeat calibration.


### 4.3 Sample measurement

#### 4.3.1 Conductivity measurement

- Place the conductivity electrode in the sample, wait 10-15s, then press  to start the measurement.
- The measurement icon  appears on the display. The measurement icon is blinking during measurement and the display shows the conductivity of the sample.
- When it reaches endpoint (auto endpoint or manual endpoint), you can record the result.

**Stability criterion for conductivity measurement:** The sensor input signal of the meter may not change by more than 0.4% from the measured average conductivity of the electrode in 6 seconds.

#### 4.3.2 TDS, Salinity or Resistivity measurement


- Press  to switch between **conductivity, TDS, Salinity and Resistivity measurement mode**.
- Follow the same procedure as for conductivity measurement.


Ohaus conductivity electrodes STCON3 and STCON7 already have a built-in temperature sensor to measure the temperature automatically.

## 5 Using the memory





### 5.1 Storing a reading

The STARTER 3100M can store up to 99 pH endpoint results and another 99 conductivity endpoint results.




- Press button  when the measurement reaches endpoint. **M01** indicates that one result has been stored.

If you press  when **M99** is displayed, **FUL** displays to indicate the memory is full. To store further data you will have to clear the memory. (See 4.4.3)



### 5.2 Recalling from memory

- Press and hold  to recall the stored values from memory when the current measurement reaches endpoint.
- Press button  or  to scroll through the stored results. **R01** to **R99** indicates which result is being displayed.
- Press  to exit.

### 5.3 Clearing the memory

- Press  or  to scroll through the stored results until “**MRCL**” appears.
- Press , **CLr** blinks;

There are now 2 options:

- ❖ Press  to confirm the deletion of all the stored data.
- ❖ Press  to return to the measurement mode without deleting the memory.

## 6 Printing

If the printer is connected to the STARTER 3100M (e.g. SF-F40A) green light means connection success.

Printer baud rate 9600bps; 8 data bit; none parity bit; 1 stop bit,

A print-out is automatically generated after each end pointed measurement or calibration.

## EN-18

## STARTER 3100M Bench Meter

### When ST3100M is in pH parameter:

The format for the print-out following a pH measurement is:

End Point, Value, Temp., ATC/MTC

Auto EP, 4.01pH, 25.0°C, MTC

The details for the second line are:

Auto EP, 4.01pH, 25.0°C, MTC

```
|-----|-----|-----|----- Manual Temperature Compensation
|-----|-----|-----|----- Temperature value and unit °C
|-----|-----|-----|----- pH value
|-----|-----|-----|----- Auto End Point
```

The format for the print-out following a mV measurement is:

End Point, Value, Temp., ATC/MTC

Auto EP, 182mV, 23.2°C, ATC

The print-out in case of an error message is:

End Point, Value, Temp., ATC/MTC

Error3

The print-out for a 2-point calibration is:

Buffer1: 4.01pH

mV1: 178mV

Temp.1: 25.0°C

Buffer2: 7.00pH

mV2: 3mV

Temp.2: 25.0°C

Slope: 99%

Offset: 5mV

ATC/MTC: MTC

The print-out for a 3-point calibration is:

Buffer1: 4.01pH

mV1: 178mV

Temp.1: 25.0°C

Buffer2: 7.00pH

mV2: 0mV

Temp.2: 25.0°C

Buffer3: 9.21pH

mV3: -130mV

Temp.3: 25.0°C

Slope: 100%

Offset: 0mV

ATC/MTC: ATC

Printing from memory:

When scrolling through the memory you can print the entry that is currently viewed by pressing



and holding(3 seconds) . The printout format is as follows:

Recall 01:

End Point, Value, Temp., ATC/MTC

Auto EP, 4.01pH, 35.6°C, ATC

**When ST3100M is in conductivity parameter:**

The format for the print-out following a Cond. measurement is:

End Point, Value, Temp., ATC/MTC  
 Auto EP, 68.8µS/cm, 26.8°C , ATC  
 Ref.25°C , T.Comp.Coeff. 2.00%/°C

The details for the second line are:

Auto EP, 85.1µS/cm, 26.8°C, ATC  
 | | | |---- Auto Temp. Compensation  
 | | |-----Temperature value and unit  
 | |----- Conductivity value  
 |----- Auto End Point

The details for the third line are:

Ref.25°C , T.Comp.Coeff. 2.00%/°C  
 | |  
 | |----- Temperature compensation coefficient value  
 |----- Reference temperature, 20 or 25 °C

The format for the print-out following a TDS measurement is:

End Point, Value, Temp., ATC/MTC  
 Auto EP, 38.0mg/L, 23.2°C , ATC  
 Ref.25°C , T.Comp.Coeff. 2.00%/°C  
 TDS-F 0.5

The format for the print-out following a Salinity measurement is:

End Point, Value, Temp., ATC/MTC  
 Auto EP, 0.08psu, 25.0°C , MTC  
 The print-out in case of an error message is:  
 End Point, Value, Temp., ATC/MTC  
 Error4

The print-out for a successful calibration is:

Standard: 1413µS/cm  
 Temperature: 30.0 °C  
 Calibration value: 1552µS/cm  
 Cell Constant: 1.66 cm-1  
 ATC/MTC: ATC

Printing from memory:

When scrolling through the memory you can print the entry that is currently viewed by pressing



and holding for 2 seconds. The printout format is followings:

Recall 08:  
 EndPoint, Value, Temp., ATC/MTC  
 Auto EP, 68.8µS/cm, 26.8°C , ATC  
 Ref.25°C , T.Comp.Coeff. 2.00%/°C

## 7 MAINTENANCE

### 7.1 Error message

#### When ST3100M is in pH mode:

Error 0	Memory access error	Reset to factory settings
Error 1	Self-diagnosis failed	Repeat the self-diagnosis procedure and make sure that you finish pressing all five keys within two minutes
Error 2	Measured values out of range	Check if the electrode is properly connected and placed in the sample solution.
Error 3	Measured buffer temperature out of range (<5 or >40 °C)	Keep the pH buffer temperature within the range for calibration
Error 4	Offset out of range offset > 60mV or < - 60 mV	Make sure the pH buffer is correct and fresh; Clean or replace the pH electrode.
Error 5	Slope out of range	Make sure the buffer is correct and fresh; Clean or replace the pH electrode.
Error 6	Meter cannot recognize the buffer	Make sure the buffer is correct and fresh; check if the buffer has not been used more than once.
Error 9	The current data set has already been stored once	An endpoint reading can only be stored once. Perform a new measurement to store.
Error 10	The sample temperature is out of range	Check the sample temperature, the temperature sensor.

#### When ST3100M is in conductivity mode:

Error 0	Memory access error	Reset to factory settings
Error 1	Self-diagnosis failed	Repeat the self-diagnosis procedure and make sure that you finish pressing all five keys within two minutes.
Error 2	Measured values out of range C: > 199.9 mS/cm TDS: < 0.1 mg/L or > 199.9 g/L SAL: > 100.0 psu	Make if the electrode is properly connected and placed in the sample solution
Error 3	Measured standard temperature out of range (5 ... 35 °C)	Keep the standard temperature within the range for calibration
Error 4	Measuring temperature out of range (0 ... 100 °C)	Check if the electrode is properly connected and keep the sample temperature within the range
Error 9	The current data set has already been stored once	An endpoint reading can only be stored once. Perform a new measurement to store.

If an error occurs, the meter will also **beep 3 times** to alert.

For further technical support please contact Ohaus. (US please contact 1-800-672-7722).

## 7.2 Meter maintenance



Never unscrew the two halves of the housing!

The STARTER 3100M series instruments do not require any maintenance other than occasional wipe with a damp cloth and the replacement of depleted batteries.

The housing is made of acrylonitrile butadiene styrene (ABS). This material is attacked by some organic solvents, such as toluene, xylene and methyl ethyl ketone (MEK). Any spillage should be immediately wiped off.

About the maintenance of the pH electrode or conductivity electrode, please see the electrode manual instructions.

## 7.3 Self-diagnosis

- When the meter is on, press and hold  and  simultaneously until the meter displays the full screen. Each icon blinks one after the other.

This way you may check whether all icons are correctly shown. The next step is to check that the keys are functioning correctly. This requires user interaction.






When **b** blinks, five icons are displayed.

- Press the five keys in any order. Each time you press a key an icon disappears from the screen, continue to press the other keys until all the icons have disappeared.

When the self-diagnosis has been completed successfully, **PAS** appears. If self-diagnosis fails, error message **Err 1** appears.

**Note:** You have to finish pressing all five keys within **2 minutes**, otherwise **Err 1** appears and you will have to repeat the procedure.

## 7.4 Recover factory settings

- When the meter is off, press and hold  &  &  simultaneously for 3 seconds, the screen displays **RSF** and blinks, this means "Reset". There are 2 options:
  - Press  to reset factory settings (MTC, slope and offset, etc.), display **YES** then restart the meter.
  - Or press  to quit the setting, the screen displays **NO** and the meter is then turned off.

## 8 TECHNICAL DATA

### 8.1 Specifications

#### Ambient conditions

- Indoor use only
- Altitude: Up to 2000 m
- Specified Temperature range: 5°C to 40°C
- Humidity: maximum relative humidity 80 % for temperatures up to 30°C decreasing linearly to 50% relative humidity at 40°C
- Mains supply voltage fluctuations: up to  $\pm 10\%$  of the nominal voltage
- Installation category II
- Pollution degree: 2
- Operability is assured at ambient temperatures between 5°C to 40°C

Spec.		ST3100M
Measurement Range	pH	-2.00...20.00 pH
	mV	-2000...+2000mV
	Conductivity	0.0 $\mu\text{S}/\text{cm}$ ...199.9mS/cm
	TDS	0.1mg/l...199.9 g/l(TDS)
	Resistivity	0...20M $\Omega$ •cm
	Salinity	0-100 psu
	Temperature	-5°C...110 °C
Resolution	pH	0.01pH
	mV	1mV
	Conductivity	0.01 $\mu\text{S}/\text{cm}$ Auto range
	TDS	0.01 mg/L Auto range
	Resistivity	0.01 $\Omega$ •cm Auto range
	Salinity	0.01 psu
	Temperature	0.1 °C
Error Limits/Accuracy	pH	$\pm 0.01$ pH
	mV	$\pm 1$ mV
	Conductivity etc.	$\pm 0.5$ %F.S.
	Temperature	$\pm 0.3$ °C
Calibration	pH	Up to 3 point, 6 buffer groups
	Conductivity	5 predefined conductivity standard points
Memory		99 sets pH and 99 sets conductivity data, last calibration data

## STARTER 3100M Bench Meter

EN-23

Power/Battery		AC Adapter Input: 100-240V ~ X.XA 50/60 Hz AC Adapter Output: 12V $\subset$ X.XA
Size/weight		Approximately 220 W x 175 D x 78 H mm / 0.95 kg
Display		LCD with backlight
Input	pH	BNC, impedance >10e+12 $\Omega$
	Conductivity	Mini-Din
	Temperature	Cinch, NTC 30 k $\Omega$
Data		RS232
Temp Compensation		ATC or MTC
Temp Compensation Range	pH	0 $^{\circ}$ C...100 $^{\circ}$ C for pH
	Conductivity	Temperature Coefficient range: 0.00 %/ $^{\circ}$ C...10.00 %/ $^{\circ}$ C
		Ref T: 20 or 25 $^{\circ}$ C
Housing		ABS

### 8.2 Compliance



This product conforms to the EMC Directive 2004/108/EC and the Low Voltage Directive 2006/95/EC. The Declaration of Conformity is available online at [europe.ohaus.com/europe/en/home/support/compliance.aspx](http://europe.ohaus.com/europe/en/home/support/compliance.aspx).



In conformance with the European Directive 2002/96/EC on Waste Electrical and Electronic Equipment (WEEE) this device may not be disposed of in domestic waste. This also applies to countries outside the EU, per their specific requirements. Please dispose of this product in accordance with local regulations at the collecting point specified for electrical and electronic equipment. If you have any questions, please contact the responsible authority or the distributor from which you purchased this device. Should this device be passed on to other parties (for private or professional use), the content of this regulation must also be related. Disposal instructions in Europe are available online at [europe.ohaus.com/europe/en/home/support/weee.aspx](http://europe.ohaus.com/europe/en/home/support/weee.aspx). Thank you for your contribution to environmental protection.

**FCC Note:** This equipment has been tested and found to comply with the limits for a Class A digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause harmful interference to radio communications. Operation of this equipment in a residential area is likely to cause harmful interference in which case the user will be required to correct the interference at his own expense.

#### ISO 9001 Registration

In 1994, OHAUS Corporation, USA, was awarded a certificate of registration to ISO 9001 by Bureau Veritas Quality International (BVQI), confirming that the OHAUS quality management system is compliant with the ISO 9001 standards requirements. On June 21, 2012, OHAUS Corporation, USA, was re-registered to the ISO 9001:2008 standard.

## 9 Appendix

### 9.1 pH Buffer Groups

STARTER 3100M automatically correct for the temperature dependence of the buffer group pH value given in the following tables (**b2, b3, b4, b5, b6**), you can find **b1** in 3.1.2 .

#### Buffer group **b2** Europe standard

Temp °C	pH2.00	pH4.01	pH7.00	pH9.21	pH11.00
5	2.02	4.01	7.09	9.45	11.72
10	2.01	4.00	7.06	9.38	11.54
15	2.00	4.00	7.04	9.32	11.36
20	2.00	4.00	7.02	9.26	11.18
<b>25</b>	<b>2.00</b>	<b>4.01</b>	<b>7.00</b>	<b>9.21</b>	<b>11.00</b>
30	1.99	4.01	6.99	9.16	10.82
35	1.99	4.02	6.98	9.11	10.64
40	1.98	4.03	6.97	9.06	10.46
45	1.98	4.04	6.97	9.03	10.28
50	1.98	4.06	6.97	8.99	10.10

#### Buffer group **b3** MERCK (Ref. 20°C)

Temp °C	pH 2.00	pH4.00	pH7.00	pH9.00	pH12.00
5	2.01	4.04	7.07	9.16	12.41
10	2.01	4.02	7.05	9.11	12.26
15	2.00	4.01	7.02	9.05	12.10
20	2.00	4.00	7.00	9.00	12.00
<b>25</b>	<b>2.00</b>	<b>4.01</b>	<b>6.98</b>	<b>8.95</b>	<b>11.88</b>
30	2.00	4.01	6.98	8.91	11.72
35	2.00	4.01	6.96	8.88	11.67
40	2.00	4.01	6.95	8.85	11.54
45	2.00	4.01	6.95	8.82	11.44
50	2.00	4.00	6.95	8.79	11.33

#### Buffer group **b4** DIN (19267) (Ref. 25°C)

Temp °C	pH1.09	pH4.65	pH6.79	pH9.23	pH12.75
5	1.08	4.67	6.87	9.43	13.63
10	1.09	4.66	6.84	9.37	13.37
15	1.09	4.66	6.82	9.32	13.16
20	1.09	4.65	6.80	9.27	12.96
<b>25</b>	<b>1.09</b>	<b>4.65</b>	<b>6.79</b>	<b>9.23</b>	<b>12.75</b>
30	1.10	4.65	6.78	9.18	12.61
35	1.10	4.65	6.77	9.13	12.45
40	1.10	4.66	6.76	9.09	12.29
45	1.10	4.67	6.76	9.04	12.09
50	1.11	4.68	6.76	9.00	11.98

**Buffer group b5 JJG119**

Temp °C	pH1.68	pH4.00	pH6.86	pH9.18	pH12.46
5	1.67	4.00	6.95	9.39	13.21
10	1.67	4.00	6.92	9.33	13.01
15	1.67	4.00	6.90	9.28	12.82
20	1.68	4.00	6.88	9.23	12.64
<b>25</b>	<b>1.68</b>	<b>4.00</b>	<b>6.86</b>	<b>9.18</b>	<b>12.46</b>
30	1.68	4.01	6.85	9.14	12.29
35	1.69	4.02	6.84	9.11	12.13
40	1.69	4.03	6.84	9.07	11.98
45	1.70	4.04	6.83	9.04	11.83
50	1.71	4.06	6.83	9.02	11.70

**Buffer group b6 J IS Z 8802 (Japanese)**

Temp °C	pH1.68	pH4.01	pH6.86	pH9.18
5	1.67	4.00	6.95	9.40
10	1.67	4.00	6.92	9.33
15	1.67	4.00	6.90	9.28
20	1.68	4.00	6.88	9.23
<b>25</b>	<b>1.68</b>	<b>4.01</b>	<b>6.86</b>	<b>9.18</b>
30	1.68	4.02	6.85	9.14
35	1.69	4.02	6.84	9.10
40	1.69	4.04	6.84	9.07

**9.2 Conductivity standards**

T(°C)	10 µS/cm	84 µS/cm	500µS/cm	1413µS/cm	12.88 mS/cm
<b>5</b>	6.1 µS/cm	53 µS/cm	315.3µS/cm	896 µS/cm	8.22 mS/cm
<b>10</b>	7.1 µS/cm	60 µS/cm	359.63µS/cm	1020 µS/cm	9.33 mS/cm
<b>15</b>	8.0 µS/cm	68 µS/cm	402.93µS/cm	1147 µS/cm	10.48 mS/cm
<b>20</b>	9.0 µS/cm	76 µS/cm	451.53µS/cm	1278 µS/cm	11.67 mS/cm
<b>25</b>	10.0 µS/cm	84 µS/cm	500.03µS/cm	1413 µS/cm	12.88 mS/cm
<b>30</b>	11.0 µS/cm	92 µS/cm	548.5µS/cm	1552 µS/cm	14.12 mS/cm
<b>35</b>	12.1 µS/cm	101 µS/cm	602.53µS/cm	1667 µS/cm	15.39mS/cm

### 9.3 Examples of temperature coefficients ( $\alpha$ -value)

Substance at 25 °C	Concentration [%]	Temperature coefficient $\alpha$ [%/°C]
HCl	10	1.56
KCl	10	1.88
CH <sub>3</sub> COOH	10	1.69
NaCl	10	2.14
H <sub>2</sub> SO <sub>4</sub>	10	1.28
HF	1.5	7.20

$\alpha$ -coefficients of conductivity standards for a calculation to a reference temperature of 25°C

Standard	Measurement temp.: 15°C	Measurement temp.: 20°C	Measurement temp.: 30°C	Measurement temp.: 35°C
84 $\mu$ S/cm	1.95	1.95	1.95	2.01
1413 $\mu$ S/cm	1.94	1.94	1.94	1.99
12.88 mS/cm	1.90	1.89	1.91	1.95

### 9.4 Conductivity to TDS conversion factors

Conductivity At 25 °C	TDS KCl		TDS NaCl	
	ppm value	Factor	ppm value	Factor
84 $\mu$ S	40.38	0.5048	38.04	0.4755
447 $\mu$ S	225.6	0.5047	215.5	0.4822
1413 $\mu$ S	744.7	0.527	702.1	0.4969
1500 $\mu$ S	757.1	0.5047	737.1	0.4914
8974 $\mu$ S	5101	0.5685	4487	0.5000
12.88 $\mu$ S	7447	0.5782	7230	0.5613
15 $\mu$ S	8759	0.5839	8532	0.5688
80 mS	52.168	0.6521	48.384	0.6048

#### LIMITED WARRANTY

Ohaus products are warranted against defects in materials and workmanship from the date of delivery through the duration of the warranty period. During the warranty period Ohaus will repair, or, at its option, replace any component(s) that proves to be defective at no charge, provided that the product is returned, freight prepaid, to Ohaus.

This warranty does not apply if the product has been damaged by accident or misuse, exposed to radioactive or corrosive materials, has foreign material penetrating to the inside of the product, or as a result of service or modification by other than Ohaus. In lieu of a properly returned warranty registration card, the warranty period shall begin on the date of shipment to the authorized dealer. No other express or implied warranty is given by Ohaus Corporation. Ohaus Corporation shall not be liable for any consequential damages.

As warranty legislation differs from state to state and country to country, please contact Ohaus or your local Ohaus dealer for further details.