

Instruction Manual

Benchtop pH/ORP/ION/Conductivity Meters
Environmental Express Series 2000



■ Preface

This manual describes the operation of the following instrument.

Brand:	Environmental Express
Series name:	Environmental Express Series 2000 Benchtop Meters
Model:	Environmental Express PH2000, Environmental Express ION2000, Environmental Express EC2000, and Environmental Express PC2000
Model description:	pH/ORP/Ion/Conductivity Benchtop Meter

Be sure to read this manual before using the product to ensure proper and safe operation of the product. Also, safely store the manual so it is readily available whenever necessary. Product specifications and appearance as well as the contents of this manual are subject to change without notice.

• Warranty and responsibility

Cole-Parmer Instrument Company warrants that the product shall be free from defects in material and workmanship and agrees to repair or replace free of charge, at option of Cole-Parmer Instrument Company, any malfunctioned or damaged product attributable to responsibility of Cole-Parmer Instrument Company for a period of three (3) years from the delivery unless otherwise agreed in a written statement. In any one of the following cases, none of the warranties set forth herein shall be extended:

- Any malfunction or damage attributable to improper operation
- Any malfunction attributable to repair or modification by any person not authorized by Cole-Parmer Instrument Company
- Any malfunction or damage attributable to the use in an environment not specified in this manual
- Any malfunction or damage attributable to violation of the instructions in this manual or operations in the manner not specified in this manual
- Any malfunction or damage attributable to any cause or causes beyond the reasonable control of Cole-Parmer Instrument Company such as natural disasters
- Any deterioration in appearance attributable to corrosion, rust and so on
- Replacement of consumables

Cole-Parmer Instrument Company SHALL NOT BE LIABLE FOR ANY DAMAGES RESULTING FROM ANY MALFUNCTIONS OF THE PRODUCT, ANY ERASURE OF DATA, OR ANY OTHER USES OF THE PRODUCT.

• Trademarks

- Microsoft, Windows, Windows Vista are registered trademarks or trademarks of Microsoft Corporation in the United States and other countries.

CODE:3200928091 - GZ0000657564

October, 2021 © 2021 Cole-Parmer Instrument Company

MEMO

- Other company names and brand names are either registered trademarks or trademarks of the respective companies. (R), (TM) symbols may be omitted in this manual.

Regulations

■ Regulations

• EU and UK Regulations

• Conformable Standards

This equipment conforms to the following standards:



EMC: EN61326-1
Class B, Basic electromagnetic environment
Safety: EN61010-1
RoHS: EN IEC 63000
9. Monitoring and control instruments including industrial monitoring and control instruments



EMC: BS EN 61326-1
Class B, Basic electromagnetic environment
Safety: BS EN 61010-1
RoHS: BS EN IEC 63000
9. Monitoring and control instruments including industrial monitoring and control instruments

Warning: This product is not intended for use in industrial environments. In an industrial environment, electromagnetic environmental effects may cause the incorrect performance of the product in which case the user may be required to take adequate measures.

• Installation Environment:

This product is designed for the following environment.


- Overvoltage category II
- Pollution degree 2
- Maximum operating altitude : 2000 m above sea level
- Range of application : For indoor use

Regulations

• Information on disposal of electrical and electronic equipment and disposal of batteries and accumulators

The crossed out wheeled bin symbol with underbar shown on the product or accompanying documents indicates the product requires appropriate treatment, collection and recycle for waste electrical and electronic equipment (WEEE) under the Directive 2012/19/EU, and/or waste batteries and accumulators under the Directive 2006/66/EC in the European Union. The symbol might be put with one of the chemical symbols below. In this case, it satisfies the requirements of the Directive 2006/66/EC for the object chemical. This product should not be disposed of unsorted household waste. Your correct disposal of WEEE, waste batteries and accumulators will contribute to reducing wasteful consumption of natural resources, and protecting human health and the environment from potential negative effects caused by hazardous substance in products.

Contact your supplier for information on applicable disposal methods.

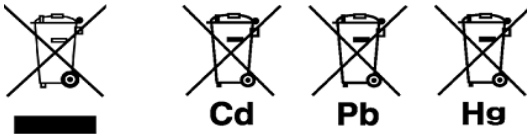

• Authorised Representative in EU

Cole-Parmer GmbH
Futtererstraße 16
Wertheim 97877
Germany
Tel: +49 9377 92030
Fax: +49 9377 1388
E-mail: sales@coleparmer.de
Website: www.coleparmer.de

• Authorized Representative in UK

Cole-Parmer Instrument Company UK
9 Orion Court Ambuscade Road
Colmworth Business Park St. Neots
Cambridgeshire PE19 8YX
United Kingdom
Tel: +44 (0)1480 272279
Free Call: +44 (0)1480 272279
E-mail: sales@coleparmer.co.uk
Website: www.coleparmer.co.uk

• FCC Rules

FCC Compliance Statement

This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

Regulations

Responsible Party for FCC matter

Oakton Instruments
625 East Bunker Court,
Vernon Hills, IL, 60061, USA
Tel: 1-888-462-5866

Note

This equipment has been tested and found to comply with the limits for a Class A digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause harmful interference to radio communications. Operation of this equipment in a residential area is likely to cause harmful interference in which case the user will be required to correct the interference at his own expense.

Any changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

■ For Your Safety

- **Hazard classification and warning symbols**

Warning messages are described in the following manner. Read the messages and follow the instructions carefully.

- **Hazard classification**



This indicates an imminently hazardous situation which, if not avoided, will result in death or serious injury. This is to be limited to the most extreme situations.



This indicates a potentially hazardous situation which, if not avoided, could result in death or serious injury.



This indicates a potentially hazardous situation which, if not avoided, may result in minor or moderate injury. It may also be used to alert against unsafe practices.

- **Warning symbols**



Description of what should be done, or what should be followed.



Description of what should never be done, or what is prohibited.

• [DEU] Sicherheitsinformation

Lesen Sie vor der Verwendung des Produkts unbedingt diese Anleitung, um den ordnungsgemäßen und sicheren Betrieb des Produkts zu gewährleisten. Bewahren Sie die Anleitung sicher auf, damit sie bei Bedarf jederzeit zur Hand ist. Die Inhalt dieser Anleitung können ohne Vorankündigung geändert werden.

• Installationsumgebung

Dieses Produkt ist nicht zum Gebrauch in industriellen Umgebungen, wie in EN61326-1 definiert, vorgesehen.

In einer industriellen Umgebung können die elektromagnetischen Störungen eventuell zu Produktfehlfunktionen führen. Um dieses Produkt unter solchen Umständen verwenden zu können, muss der Benutzer ggf. angemessene Maßnahmen ergreifen.

Das Produkt ist gemäß EN61010-1 für die folgende Umgebung vorgesehen.

- Überspannungskategorie II
- Verschmutzungsgrad 2

• [FRA] Informations de sécurité

Veillez à lire le présent manuel avant d'utiliser le produit de manière à garantir son utilisation correcte et sûre.

De même, rangez le manuel dans un lieu sûr de manière à pouvoir vous y reporter lorsque cela est nécessaire.

Le contenu du présent manuel peut être modifié sans notification préalable.

• Environnement d'installation

Ce produit n'est pas destinés à une utilisation dans des environnements industriels, tels que définis dans la norme EN61326-1.

Dans un environnement industriel, les interférences électromagnétiques peuvent entraîner un dysfonctionnement du produit. Pour utiliser le produit dans ce type d'environnements, l'utilisateur peut avoir à prendre des mesures appropriées.

Le produit est conçu pour l'environnement suivant, tel que défini dans la norme EN61010-1.

- Catégorie de surtension II
- Degré de pollution 2

• [ITA] Informazioni sulla sicurezza

Leggere attentamente questo manuale prima di utilizzare il prodotto al fine di utilizzarlo in modo sicuro e adeguato. Inoltre, conservare in un luogo sicuro il manuale per poterlo consultare se necessario.

Le contenuti di questo manuale sono soggetti a modifiche senza preavviso.

• Ambiente di installazione

Questo prodotto non è stato progettato per essere utilizzato in ambienti industriali, secondo la norma EN61326-1.

In un ambiente industriale, le interferenze elettromagnetiche potrebbero causare un malfunzionamento del prodotto. Per utilizzare il prodotto in tali ambienti, all'utente potrebbe essere richiesto di adottare le contromisure necessarie.

Il prodotto è designato per il seguente ambiente, definito nello standard EN61010-1.

- Categoria di sovratensione II
- Livello di inquinamento 2

• [SWE] Säkerhetsinformation

Se till att du läser denna handbok innan du börjar använda produkten för en korrekt och säker användning av den. Spara sedan handboken på en säker och lättåtkomlig plats så att du kan konsultera den när så behövs.

Innehållet i denna handbok kan komma att ändras utan föregående meddelande därom.

• Installationsmiljö

Detta produkten är ej avsedda för användning i industriella miljöer enligt riktlinjerna i EN61326-1.

Om den används i industrimiljöer kan de elektromagnetiska störningarna orsaka tekniska fel hos produkten. Om produkten ska användas i sådana miljöer kan användaren behöva vidta lämpliga åtgärder för att lösa dessa problem.

Produkten är utformad för användning i följande miljöer, i enlighet med SS-EN 61010-1.

- Överspänningskategori II
- Föroreningsgrad 2

• [SPA] Información de seguridad

Asegúrese de leer este manual antes de utilizar el producto para garantizar un uso correcto y seguro del mismo. Asimismo, guarde de forma segura el manual para que esté disponible siempre que sea necesario.

El contenido de este manual están sujetos a cambios sin previo aviso.

• Entorno de instalación

Este producto está diseñado para su uso en entornos industriales, tal y como se define en EN61326-1.

En un entorno industrial, las interferencias electromagnéticas pueden provocar un funcionamiento

incorrecto del producto. Para usar el producto en tales entornos, el usuario debe tomar las medidas adecuadas.

El producto se ha diseñado para el siguiente entorno, definido en EN61010-1.

- Categoría de sobretensión II
- Nivel de contaminación 2

• [POL] Informacje dotyczące bezpieczeństwa

Przed przystąpieniem do użytkowania tego produktu należy dokładnie zapoznać się z niniejszą instrukcją, aby zapewniona była prawidłowa i bezpieczna eksploatacja produktu. Instrukcję przechowywać w bezpiecznym miejscu, aby w razie potrzeby była zawsze dostępna.

Treść niniejszej instrukcji może ulec zmianie bez wcześniejszego powiadomienia.

• Środowisko instalacji

Ten produkt nie są przeznaczone do użytkowania w środowisku przemysłowym, zgodnie z definicją określoną w normie EN61326-1.

W środowisku przemysłowym zakłócenia elektromagnetyczne mogą powodować nieprawidłowe działanie produktów. Możliwe, że aby użytkować produkt w takich środowiskach, użytkownik będzie musiał podjąć stosowne środki zaradcze.

Produkt jest przeznaczony do użycia w poniższym środowisku zdefiniowanym w normie EN61010-1.

- Kategoria przepięciowa II
- Stopień zanieczyszczenia 2

• [NLD] Veiligheidsinformatie

Lees deze handleiding voordat u dit product gebruikt zodat u het op de juiste manier en veilig kunt gebruiken. Bewaar de handleiding goed zodat u hem wanneer nodig kunt raadplegen.

De inhoud van deze handleiding kunnen zonder voorafgaande kennisgeving worden gewijzigd.

• Installatieomgeving

Dit product is niet bedoeld voor gebruik in een industriële omgeving zoals gedefinieerd in EN 61326-1.

In een industriële omgeving kan de elektromagnetische interferentie de werking van dit product storen. Voor gebruik van het product in een dergelijke omgeving moet de gebruiker mogelijk maatregelen treffen om de storing te verhelpen.

Het product is ontworpen voor de volgende omgeving, gedefinieerd in EN 61010-1.

- Overspanningscategorie II
- Vervuilingsgraad 2

• [JPN] 安全情報

ご使用になる前に、本書を必ずお読みください。お読みになった後は必要なときにすぐに取り出せるように大切に保管してください。

本書に記載されている内容は予告なく変更される場合があります。あらかじめご了承ください。

・設置環境

本製品は、EN61326-1 で定義される工業環境で使用することを想定した製品ではありません。

工業環境においては、電磁妨害の影響を受ける可能性があり、その場合には使用者が適切な対策を講ずることが必要となることがあります。

本製品は、EN61010-1 で定義される以下の環境用に設計されています。

- 過電圧カテゴリー II
- 汚染度 2

For Your Safety

• Safety precautions

This section provides precautions for using the product safely and correctly and to prevent injury and damage. The terms of DANGER, WARNING and CAUTION indicate the degree of immanency and hazardous situation. Read the precautions carefully as it contains important safety messages.

• Instrument and electrode



WARNING



Do not disassemble or modify the instrument. Otherwise, it may heat up or be ignited resulting in a fire or an accident.



CAUTION



Harmful chemicals

Some electrodes are used with hazardous standard solutions. Handle them with care. The internal solution of pH electrode is highly concentrated potassium chloride (3.33 mol/L KCl). If the internal solution comes in contact with the skin, wash it off immediately. If it gets into the eyes, flush with plenty of water and then consult a doctor.



Broken glass

Broken glass may cause injury. The outer tube and tip of an electrode are made of glass. Handle them with care.



Do not use the phono jack under wet or humid conditions. Otherwise, it may cause a fire, electric shock, or breakage.

Product Handling Information

■ Product Handling Information

• Operational Precautions (instrument)

- Only use the product including accessories for their intended purpose.
- Do not drop or physically impact the instrument.
- The instrument is made of solvent-resistant materials but that does not mean it is resistant to all chemicals. Do not expose the instrument in strong acid or alkali solution, or wipe with such solution.
- If the instrument is dropped into water or gets wet, wipe it using soft cloth. Do not heat to dry it.
- Use fingers to press the operation keys. Do not use a hard object like a metal stick or rod.
- Be careful not to let water inside the instrument. The instrument is not waterproof.
- To disconnect an electrode or serial cable, hold the connector and pull it off. If you pull at the cable, it may cause breakage.
- The phono jack communication between the instrument and a personal computer (referred to as PC in the rest of this document) may fail because of environmental conditions, such as electromagnetic noise.
- Do not use an object with a sharp end to press the keys.
- If the power supply is interrupted while measurement data is being saved in the instrument, the data could be corrupted.
- Make sure to use the provided power supply cable to power this product.

• Environmental conditions for use and storage

- Temperature: 0°C to 45°C
- Humidity: under 80% relative humidity and free from condensation

• Avoid the following conditions:

- Strong vibration
- Direct sunlight
- Corrosive gas environment
- Locations close to an air-conditioner
- Direct wind
- Dusty Environment

• Transportation

When transporting the instrument, repackage it in the original package box. Otherwise, it may cause instrument damage.

• Disposal

- Standard solution used for the calibration must be under neutralized before the disposal.
- When disposing of the product, follow the related laws and regulations of your country for disposal of the product.

Manual Information

■ Manual Information

- Description in this manual

Note

This interprets the necessary points for correct operation and notifies the important points for handling the product.

Tip

This indicates reference information.

- **Product Overview.....1**
 - Package Content..... 1
 - Key Features..... 2
- **Basic Operations..... 6**
 - Turning On the Instrument.....6
 - Connecting an Electrode..... 6
 - Changing the Operation Mode..... 7
 - Changing the Measurement Parameter.....9
- **Calibration..... 10**
 - pH Calibration..... 10
 - ORP/mV Calibration..... 13
 - Ion Calibration..... 15
 - Conductivity Calibration.....18
 - TDS Calibration..... 21
 - Salinity Calibration.....22
 - Temperature Calibration..... 24
- **Data..... 26**
 - Data Capture and Storage..... 26
 - Data Transfer..... 27

Contents


■ Setup.....	28
• P1 pH Setup.....	28
• P1 Ion Setup.....	33
• P1 COND Setup.....	38
• P2 TDS Setup.....	45
• P3 SAL Setup.....	48
• Data Setup.....	52
• General Setup.....	56
• Clock Setup.....	62
■ Maintenance and Storage.....	65
• Contact for Maintenance.....	65
• Maintenance and Storage of the Instrument.....	65
• Maintenance and Storage of Electrodes.....	66
■ Error Messages and Troubleshooting.....	69
■ Appendix.....	74

■ Product Overview

The Environmental Express Series 2000 benchtop meters are optimized for laboratory measurement, and allow you to measure pH, ORP/mV, ion, conductivity, resistivity, TDS, salinity and temperature.

This section describes the package content, key features and product components of Environmental Express Series 2000 benchtop meters.

● Package Content

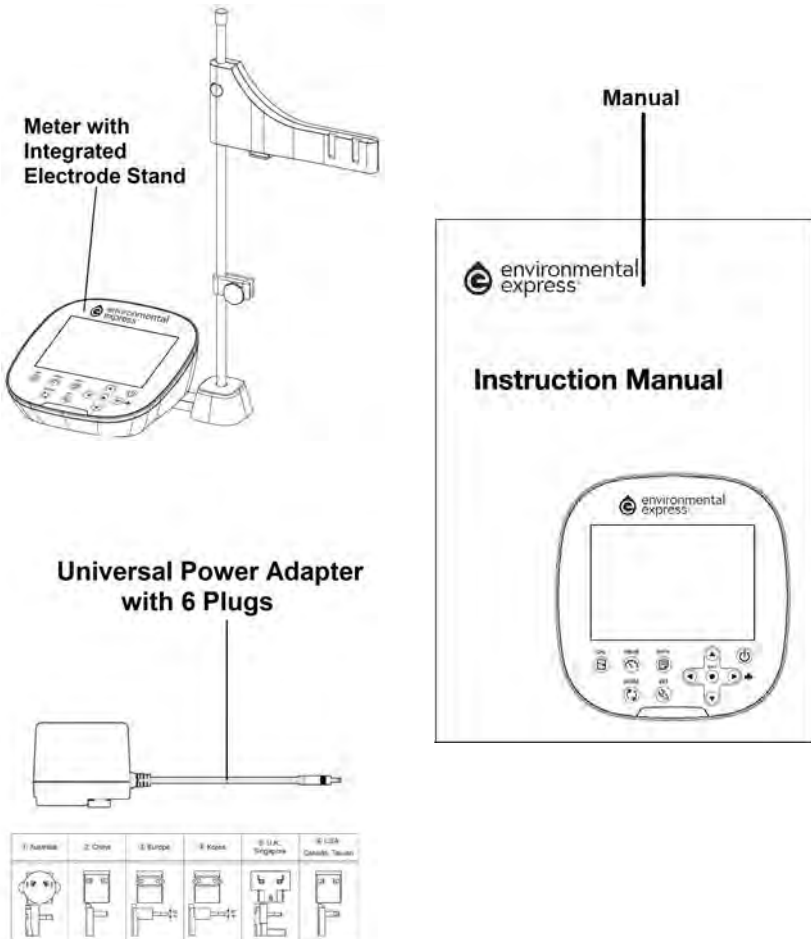


After opening the package, check for damage on the instrument and the standard accessories

all exist. If damage or defects are found on the product, contact your dealer.

● Key Features

- Large monochrome LCD
- Integrated electrode holder (up to 2 electrodes) that can be attached to either side of the meter
- Simple user interface and single parameter display
- 2000 Memory data
- Real time clock
- Automatic Temperature Compensation (ATC) with temperature calibration
- Adjustable auto shut-off time (1 to 30 minutes)
- Auto stable, auto hold, and real time measurement modes with reading stability indicators
- PC (standard USB) / printer (25 pin serial) connection via 2.5 mm diameter phono jack
- Adjustable calibration alarm (1 to 90 days)
- Auto data log with date and time stamp
- Software upgrade
- Password protection for setup mode

• Display

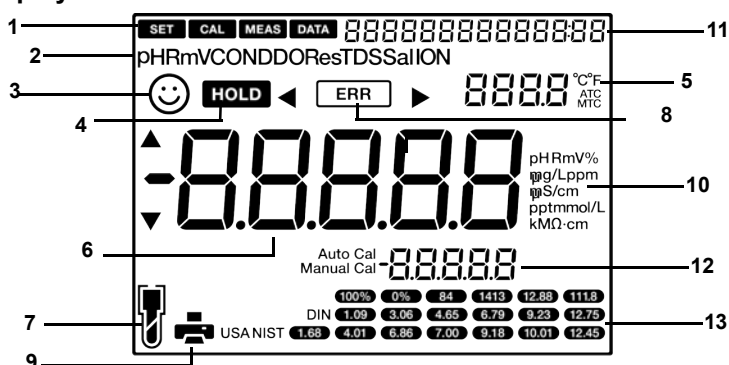

No	Name	Function
1	Status Icon	Displays the current operation mode (Setup, Calibration, Measurement and Data mode)
2	Parameters	Displays the measured parameters like pH, mV, ION, COND, Res, TDS and Sal
3		Smiley icon and sound indicate value is stable for documentation in Auto Stable and Auto Hold modes
4		Appears when the measured value display is stable and fixed in Auto Hold mode
5	Temperature Display Area	Displays the measured temperature, temperature unit, and ATC/MTC
6	Measured Value, Set Item Display Area	Displays the measured value and the set value
7		Indicates electrode sensitivity level
8		Indicates error situation
9		Indicates data being transferred to the printer or computer
10	pH RmV% µg/Lppm µS/cm ppt kMΩ·cm	Displays the unit for the measurement parameter
11	8888888888888888	Displays date and time

Product Overview


No	Name	Function
12	Auto Cal Manual Cal 	Displays the calibration method
13		Displays the pH buffer groups, pH buffer values and conductivity standards

● Electrode Sensitivity Level

Electrode Icon		pH Average Slope	Ion Average Slope	Conductivity Average Calibration Factor	Salinity Calibration Factor
	Excellent	95.0 to 105.0%	90.1 to 199.9%	0.909 to 1.111	0.9 to 1.1
	Very Good	85.0 to 94.9%	85.1 to 90.0%	0.800 to 1.250	0.8 to 1.2
	Good	80.0 to 84.9%	50.1 to 85%	0.70 to 1.43	0.7 to 1.3

If “SLPE ERR” appears, refer to page 69.

• Keypad Operation

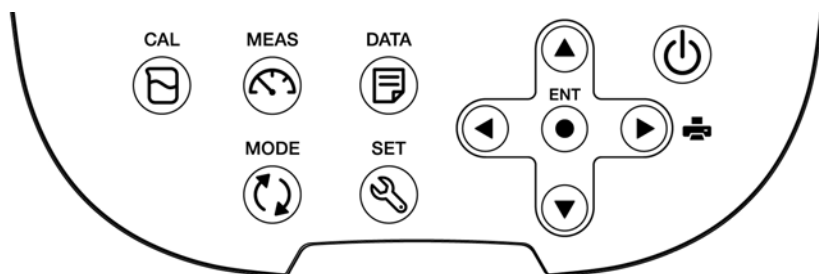


Keypad	Name	Function
	CAL key	Switches from the measurement mode to the calibration mode. Starts calibration in the calibration mode.
	MEAS key	Switches from the operation mode to the measurement mode. Releases the fixed measurement value mode in the auto hold mode and begins a fresh measurement.
	DATA key	Switches from the measurement mode to the data mode.
	MODE key	In the measurement mode, changes measurement parameters.
	SET key	Switches from the measurement mode to the setup mode.
	ENTER key	Determines the selection or setup. Saves data in the measurement mode and calibration mode.
	UP key	Navigates between various settings in setup mode. Increases or decreases selected digit when entering numbers.
	DOWN key	
	RIGHT key	Navigates between digit positions when entering numbers.
	LEFT key	Prints out the measurement values ( key).
	POWER key	Powers ON/OFF the instrument.

■ Basic Operations

This section describes the basic operations such as turning on the instrument, connecting an electrode, and changing the operation modes and measurement parameters of Environmental Express Series 2000 benchtop meters.

● Turning On the Instrument

1. Insert the AC adapter cable by fitting with the AC adapter jack.
2. Insert the AC adapter into the electrical socket.
3. Press the POWER key of the meter.

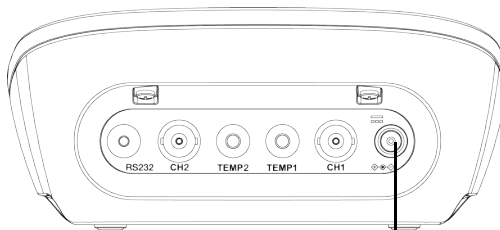


AC Adapter jack

● Connecting an Electrode

To perform calibration / measurement, it is necessary to use the appropriate electrode for measurement parameter. Use the following procedure to correctly connect the electrode to the instrument:

1. Insert the electrode connector by fitting its groove with the connector pin of the instrument.
2. Turn the electrode connector clockwise by following the grooves.
3. Slide the connector cover on the connector.
4. When using a combination electrode equipped with a temperature sensor, insert the temperature jack (T) to the ATC socket on the meter.

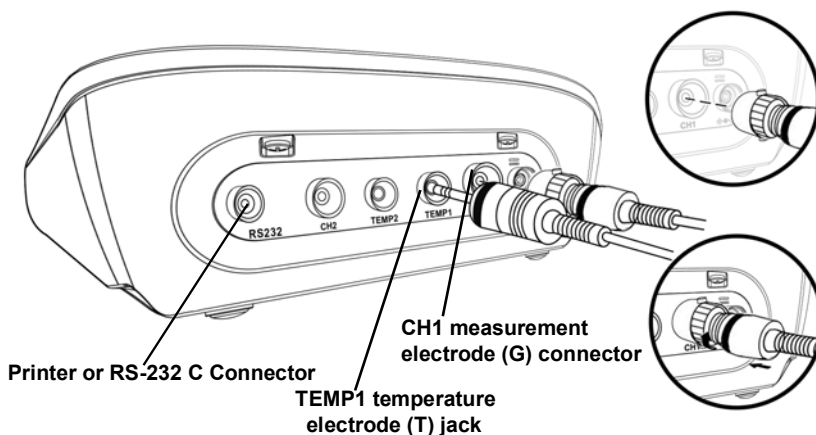

• Changing the Operation Mode

You can change the operation mode to four available modes depending on the purpose of use. The status icon indicates the current mode.




Icon	Name	Function
MEAS	Measurement mode	Performs measurement.
CAL	Calibration mode	Performs calibration.
DATA	Data mode	Displays the saved data.
SET	Setup mode	Performs various setups for different functions.

Basic Operations


You can change the operation mode using the corresponding key:

- **Measurement mode:** Press the  key to change to the measurement mode.
- **Calibration mode:** In the measurement mode, press the  key to change to the calibration mode.
- **Data mode:** In the measurement mode, press the  key to change to the data mode.
- **Setup mode:** In the measurement mode, press the  key to change to the setup mode.

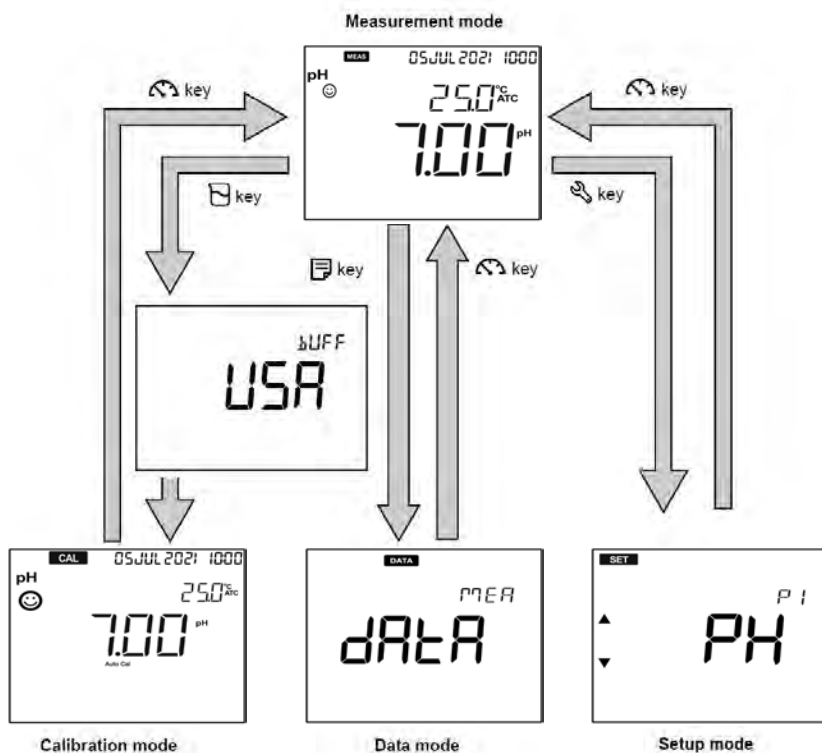

• Changing the Measurement Parameter

This instrument measures pH, ORP/mV, ion, conductivity, resistivity, TDS, and salinity. For measurement, an electrode corresponding to the measurement parameter is required. In the measurement mode, the measurement parameter can be changed by pressing the  key.

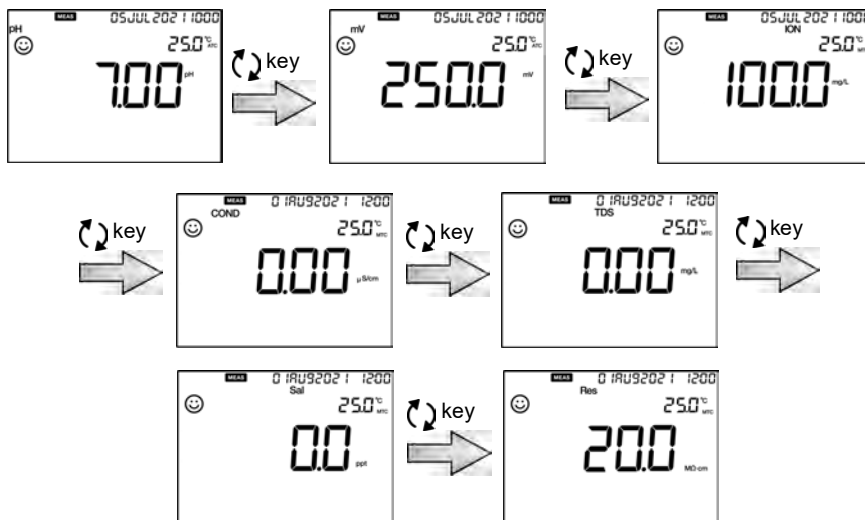

Model	Measurement Parameters
PH2000	pH, ORP/mV
ION2000	pH, ORP/mV, Ion
EC2000	Conductivity, TDS, Salinity, Resistivity
PC2000	pH, ORP/mV, Ion, Conductivity, TDS, Salinity, Resistivity

■ Calibration

This section describes the calibration procedures using Environmental Express Series 2000 benchtop meters and electrodes.

● pH Calibration

Calibration is necessary for accurate pH measurement. To perform pH calibration using Environmental Express PH2000, ION2000, or PC2000 meter, follow the procedure detailed below:

Prerequisites

- Clean the pH electrode with DI (deionized) water and wipe it with tissue paper.
- Switch on the meter and plug in the pH electrode.
- Prepare the pH buffers required for calibration.
- Keep the meter in pH measurement mode.
- Dip the pH electrode at least 3 cm in the pH buffer.

Note


- Perform two-point calibration using:
pH 7 and 4 for acidic sample.
pH 7 and 10 for alkaline sample.
 - Perform three-point calibration using pH 7, 4 and 10 if you are unsure of the expected sample pH value. It is recommended to calibrate with pH 7 first.
 - Default pH buffer group in buffer setup is **USA**. If you want to change to **NIST**, **NIST2**, **DIN**, or **CUST** (Custom) refer to “P1.1 Buffer Setup” on page 29.
 - For **USA**, **NIST**, **NIST2**, and **DIN** pH buffer groups, follow the Auto Calibration procedure. For **CUST**, follow Manual Calibration procedure.
-

Tip

- To abort an ongoing calibration process at any point of time, press the  key.
 - It is recommended to clear the previous calibration data before performing calibration. For erasing the calibration data, refer to “P1.4 Calibration Clear Setup” on page 32.
-

Auto Calibration

1. After placing the pH electrode in pH buffer, press the **CAL**  key.
2. The selected pH buffer group (**USA**, **NIST**, **NIST2** or **DIN**) appears on the meter screen and meter starts checking various calibration values with a blinking  on screen.
3. Wait for the  to stabilize. When it stabilizes, there will be a sound indicating that reading is stable.
4. Press the **ENT**  key to confirm and save calibration data.
5. Meter displays **CAL DONE** indicating end of the pH calibration procedure. Electrode icon, pH buffer group, and calibrated pH buffer icon light up in measurement mode.
6. Repeat above steps for other calibration points as required.

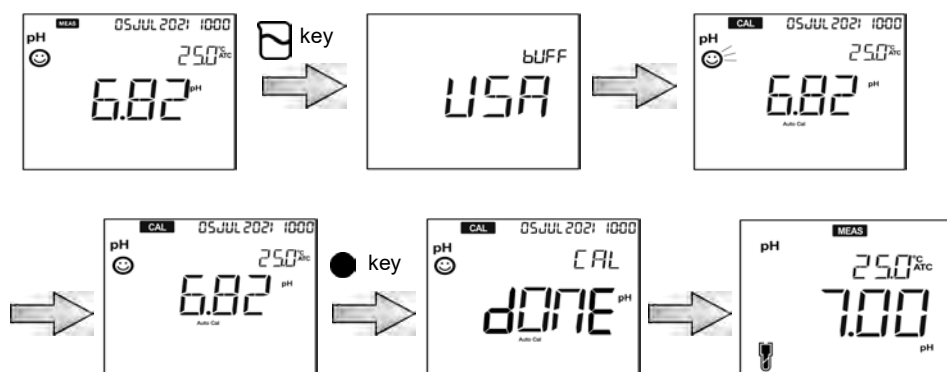


Note

To view and/or print calibration data, press the  key when you are in the **CAL** mode. The display scrolls through the calibrated values, segment slope(s), average slope, and offset.

Manual Calibration

1. After placing the pH electrode in pH buffer, press the **CAL**  key.
2. The selected **CUST** pH buffer group appears on the meter screen.
3. Wait for the  to stabilize. When it stabilizes, there will be a sound indicating that reading is stable.
4. Press   and   keys to enter the pH buffer value.
5. Press the **ENT**  key to confirm and save calibration data.
6. Meter displays **CAL DONE** indicating end of the pH calibration procedure. Electrode icon and number of calibration points done (e.g. 1 PT for 1 point, 2 PTS for 2 points) light up in measurement mode.
7. Repeat above steps for other calibration points as required.

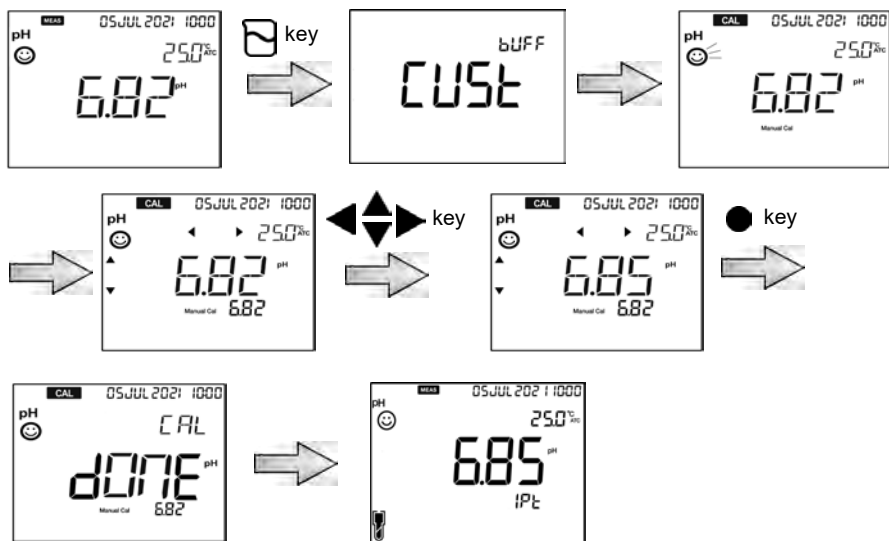

Note

To view and/or print calibration data, press the  key when you are in the **CAL** mode. The display scrolls through the calibrated values, segment slope(s), average slope, and offset.

• ORP/mV Calibration

Calibration is necessary for accurate ORP measurement. To perform ORP calibration using Environmental Express PH2000, ION2000, or PC2000 meter, follow the procedure detailed below:

Prerequisites

- Clean the ORP electrode with DI (deionized) water and wipe it with tissue paper.
- Switch on the meter and plug in the ORP electrode.
- Prepare standard solution required for calibration.
- Ensure that the meter is in mV measurement mode.
- Dip the ORP electrode into the standard solution ensuring that the solution level is at least 3 cm from the electrode tip.

Note


- Absolute value measurement mode and relative value measurement mode are the two types of measurement mode available for ORP (mV) measurement.
- In absolute value measurement mode, the handheld meter displays the actual voltage value.
- In relative value measurement mode, user can adjust the absolute mV value by calibration. If the mV value is adjusted, the meter automatically indicates relative mV value as **RmV**. The adjustment mV is applied as an offset to the absolute mV value.
- In the relative mV mode, the absolute mV value can be adjusted by ± 200 mV.

Tip

To abort an ongoing calibration process at any point of time, press the  key.

Calibration

1. After placing the ORP electrode in ORP standard solution, press the  key to switch to mV mode.
2. Press the  key.
3. Meter starts reading mV values.
4. Wait for the  to stabilize. When it stabilizes, there will be a sound indicating that reading is stable.
5. Use the   and   keys to adjust the mV value to the ORP standard solution value.
6. Press the **ENT**  key to confirm and save calibration data.
7. Meter displays **CAL DONE** indicating end of the ORP/mV calibration procedure. mV changes to RmV in measurement mode.

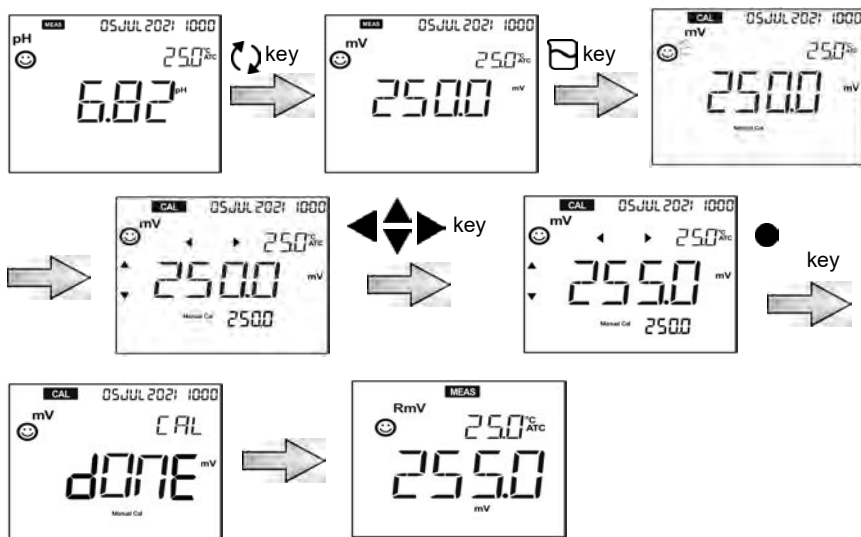

• Ion Calibration

Calibration is necessary for accurate ion measurement. To perform ion calibration using Environmental Express ION2000 or PC2000 meter, follow the procedure detailed below:

Prerequisites

- If ion electrode is new or stored for long period, condition it first. Refer to the ion electrode manual for the electrode preparation and conditioning procedures.
- Clean the ion electrode with DI (deionized) water and wipe it with tissue paper.
- Switch on the meter and plug in the ion electrode.
- Ensure that the meter is in ion measurement mode.
- Select the ion electrode in use (or set the ion valence) and concentration unit of standard solutions in ion setup mode.
- Prepare standard solutions required for calibration. Refer to the ion electrode manual for the standard solution preparation procedure.
- Dip the ion electrode into the standard solution ensuring that the solution level is at least 3 cm from the electrode tip.

Note


- For calibration, prepare at least 2 standards solutions with ionic strength adjustor that are ten-fold apart in concentration.
- Standard solutions should bracket the expected ion concentration in the sample.
- For setting the ion concentration unit, refer to "P1.1 Ion Concentration Unit Setup" on page 34. Three units are available: $\mu\text{g/L} \leftrightarrow \text{mg/L} \leftrightarrow \text{g/L}$, $\text{ppm} \leftrightarrow \text{ppt}$, and $\text{mmol/L} \leftrightarrow \text{mol/L}$.
- For selecting the ion electrode type or setting the valence of the ion to be measured, refer to "P1.2 Ion Electrode Type Setup" on page 35. Seven ion electrode types are available: **NH3** (Ammonia), **CL** (Chloride), **FL** (Fluoride), **NO3** (Nitrate), **POT** (Potassium), **CA** (Calcium) and **CUST** (Custom).
- Select **CUST** and then the correct ion valence (-2, -1, 1, 2), if the ion electrode in use is not in the selection of ion electrode types. Ion valence is **CHRG** in the meter, which stands for "charge".
- Ion concentration varies depending on the sample temperature. For accurate measurement, it is recommended that the calibration and measurement are carried out at a constant temperature (e.g., using a constant temperature bath). Stir the standard solutions and samples using a stirrer during calibration and measurement.
- Because the ion electrode is not equipped with a temperature sensor, the temperature electrode must be connected in order to use the automatic temperature compensation (ATC). In ATC mode, the Nernst slope (mV/one decade) is automatically changed corresponding to the measured temperature by the temperature sensor. If the ATC function is not used, match the temperature setting of the instrument to the temperature of the standard solutions during calibration and match the sample temperature to the temperature setting of the instrument in measurement. By doing so, you can obtain the correct measurement value without being affected by sensitivity variation caused by temperature.

Tip

- To abort an ongoing calibration process at any point of time, press the  key.
 - It is recommended to clear the previous calibration data before performing calibration. For erasing the calibration data, refer to "P1.3 Calibration Clear Setup" on page 37.
-

Calibration

1. After placing the ion electrode in standard solution, press the  key.
2. Wait for  to stabilize. When it stabilizes, there will be a sound indicating that reading is stable.
3. Press   and   keys to enter the standard solution concentration and adjust the unit. Press the  key to adjust the decimal point location.
4. Press the **ENT**  key to confirm and save calibration data.
5. Meter displays **CAL DONE** that indicates end of the ion calibration procedure. Electrode icon and number of calibration points done (e.g. 1 PT for 1 point, 2 PTS for 2 points) light up in measurement mode.
6. Repeat above steps for other calibration points as required.

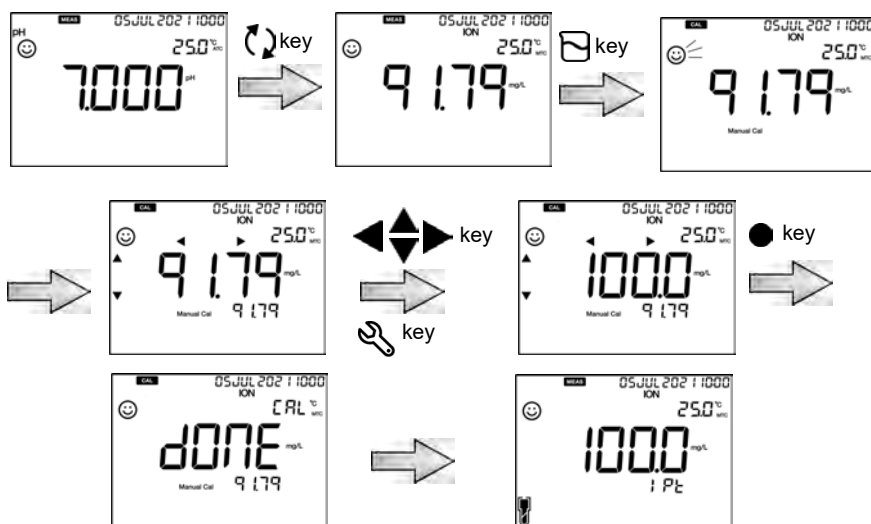

Note

To view and/or print calibration data, press the  key when you are in the **CAL** mode. The display scrolls through the calibrated values, segment slope(s) and average slope.

• Conductivity Calibration

Calibration is necessary for accurate electrical conductivity measurement. To perform conductivity calibration using Environmental Express EC2000 or PC2000 meter, follow the procedure detailed below:

Prerequisites

- Clean the conductivity electrode with DI (deionized) water and wipe it with tissue paper.
- Switch on the meter and plug in the conductivity electrode.
- Prepare conductivity standard(s) required for calibration.
- Ensure that the meter is in **COND** mode.
- Dip the conductivity electrode in the conductivity standard until the hole at the upper part of the electrode is immersed.

Note


- Salinity, TDS, and resistivity of a sample solution are calculated from the measured value of conductivity.
 - In conductivity calibration mode, the default calibration method is auto calibration. If you like to change it to manual calibration method, refer to "P1.3 Auto Calibration Setup" on page 41.
-

Tip

- For second or multiple point calibration, clean the conductivity electrode with DI water and follow the same procedure.
 - If you are performing multiple point calibration, calibrate to the lowest conductivity first and then move to increasing conductivity values. This minimizes cross contamination.
 - To abort an ongoing calibration process at any point of time, press the  key.
-

Auto Conductivity Calibration

1. After placing the conductivity electrode in the conductivity standard, press the  key.
2. Meter displays **AUTO CAL** and starts measuring various calibration values with a  blinking on screen.
3. Wait for the  to stabilize. When it stabilizes, there will be a sound indicating that reading is stable.
4. Press the **ENT**  key to confirm and save calibration data.
5. Meter displays **CAL DONE** indicating end of the conductivity calibration procedure.
Electrode icon and calibrated conductivity standard icon light up in measurement mode.
6. Repeat for other calibration points as required.
7. You can calibrate one point for each range.

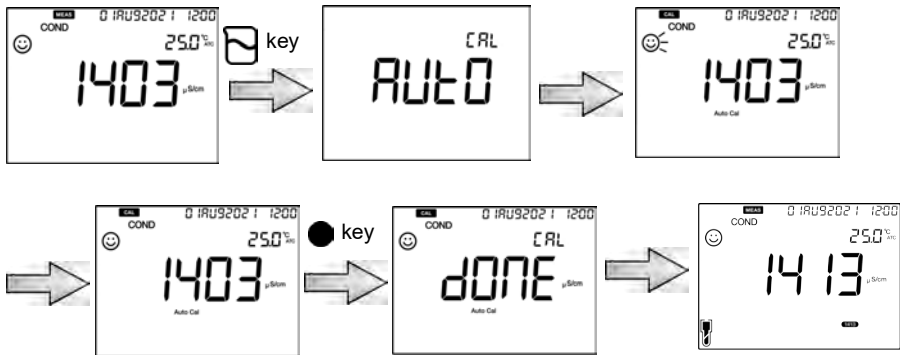


Note

To view and/or print calibration data, press the  key when you are in the **CAL** mode. The display scrolls through the calibrated conductivity standard values, calibration factors, and average calibration factor.

Manual Conductivity Calibration

1. After placing the conductivity electrode in the conductivity standard, press the  key.
2. Meter displays **MANUAL CAL** and starts measuring with a blinking  on screen.
3. Wait for the  to stabilize. When it stabilizes, there will be a sound indicating that reading is stable.
4. Use the   and   keys to enter the electrical conductivity value of the conductivity standard. Press the  key to adjust the decimal point location.
5. Press the **ENT**  key to confirm and save calibration data.
6. Meter displays **CAL DONE** indicating end of the conductivity calibration procedure. Electrode icon and number of calibration points done (e.g. 1 PT for 1 point, 2 PTS for 2 points) light up in measurement mode.
7. Repeat for other calibration points as required.
8. You can calibrate one point for each range.

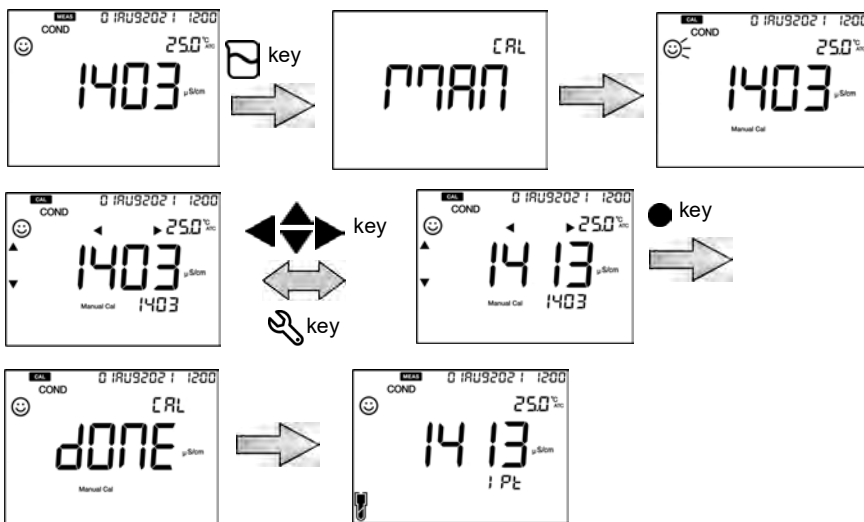

• TDS Calibration

Total dissolved solids (TDS) is calculated from the measured conductivity value so TDS calibration is not required. Once conductivity mode is calibrated, TDS values will be recalculated accordingly.

Set the appropriate TDS curve. Available TDS curves in the meter are as follows:

- **LINR** (Linear KCl curve with adjustable factor from 0.40 to 1.00)
- **442** (Myron L 442 non-linear curve)
- **EN** (European environmental standard non-linear curve)
- **NACL** (non-linear salinity curve)

Note

- The default TDS curve is **LINR**. To set a desired TDS curve, refer to "P2.1 TDS Curve Setup" on page 46.
-

● Salinity Calibration

Calibration is necessary for accurate salinity measurement. To perform salinity calibration using Environmental Express EC2000 or PC2000 meter, follow the procedure detailed below:

Prerequisites

- Clean the conductivity electrode with DI (deionized) water and wipe it with tissue paper.
- Switch on the meter and plug in the conductivity electrode.
- Prepare salinity standard required for calibration.
- Ensure that the meter is in **SAL** mode.
- Dip the conductivity electrode in the salinity standard until the hole at the upper part of the electrode is immersed.

Note


- Before salinity calibration, set the required salinity type. The available salinity types are:
 - NACL**
 - SEA.W** (Seawater)
 - The default salinity type is **NACL**. To set a desired salinity type, refer to “P3.2 Salinity Type Setup” on page 50.
 - User can adjust the salinity value by calibration.
-

Tip

To abort an ongoing calibration process at any point of time, press the  key.

Calibration

1. After placing the conductivity electrode in the salinity standard, press the  key.
2. Meter starts measuring with a  blinking on screen.
3. Wait for the  to stabilize. When it stabilizes, there will be a sound indicating that reading is stable.
4. Use the   and   keys to enter the salinity standard value.
5. Press the **ENT**  key to confirm and save calibration data.
6. Meter displays **CAL DONE** indicating end of the salinity calibration procedure. Electrode icon lights up in measurement mode.

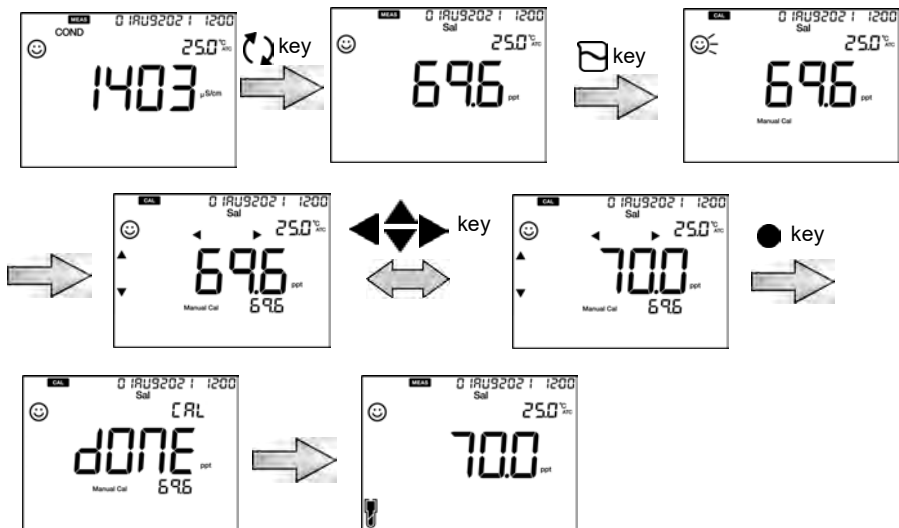

Note

To view and/or print calibration data, press the  key when you are in the **CAL** mode. The display scrolls through the calibrated salinity standard value and calibration factor.

• Temperature Calibration

Temperature calibration is required to accurately match electrode to the meter. Check the temperature reading and if it is acceptable, no temperature calibration is required. If you need to calibrate, please follow the procedure detailed below:

Prerequisites

- Clean the electrode with DI (deionized) water and wipe it with tissue paper.
- Switch on the meter and plug in the electrode and temperature sensor.
- Dip the electrode in a solution with known temperature until its temperature sensor is immersed.
- Wait for 5 minutes to ensure temperature stability.

Note


- Meter displays **MTC** if the temperature sensor is not plugged in and displays **ATC** if the temperature sensor is plugged in.
 - Temperature calibration must be performed using a solution with known temperature or against a calibrated thermometer.
-

Tip

To abort an ongoing calibration process at any point of time, press the  key.

Calibration

1. After placing the electrode in a solution with known temperature, press the  key.
2. Press the  key to switch to temperature calibration mode. Meter displays measured temperature value.
3. Use the   and   keys to adjust the temperature to the required value.
4. Press the **ENT**  key to confirm and save calibration data.
5. Meter displays **CAL DONE** indicating end of the temperature calibration procedure.

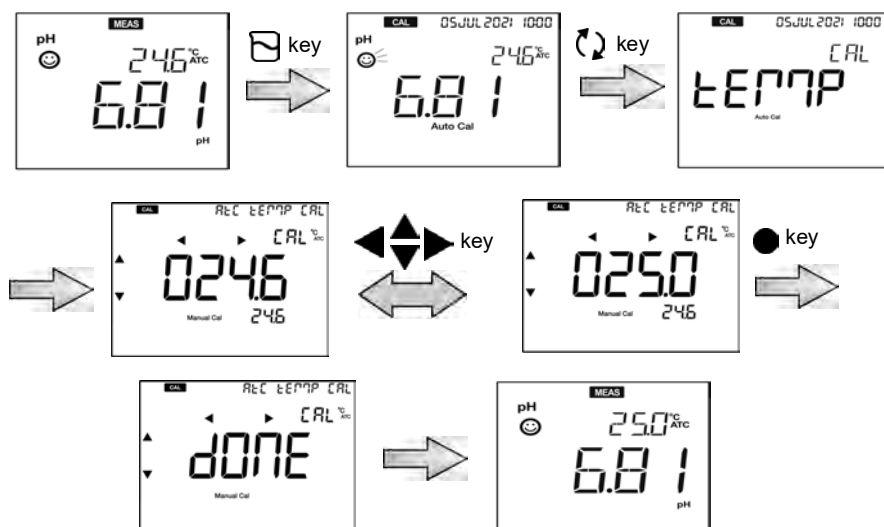

■ Data

This section describes the procedures for storing data into Environmental Express Series 2000 benchtop meters and viewing them as well as transferring data from the meter to a PC.

● Data Capture and Storage

● Storing Data

Data measured by the instrument can be stored in the internal memory.

- To save the measured data, press the **ENT**  key.
- Meter displays the location number of the saved data for 2 seconds and then the previous screen automatically.




Note

- If the data storage limit reaches 2000, memory data full error occurs and **DATA FULL** is displayed.
- In such case, print or transfer necessary data to a PC and delete the data from the internal memory of the instrument.

● Viewing Stored Data

- To view stored data, press  key .
- Use   keys to scroll through all stored data.
- Press  key to return to measurement mode.

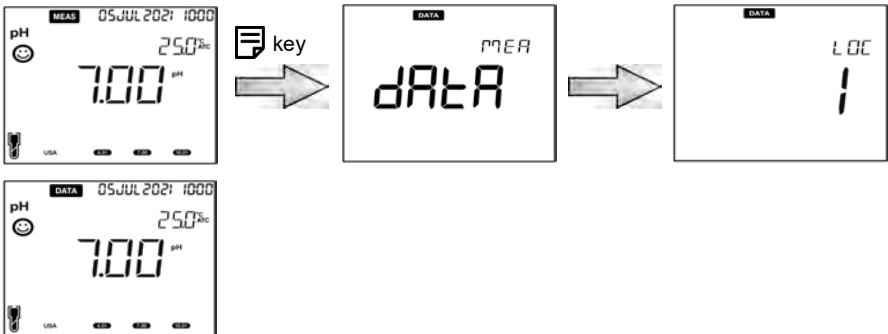

• Data Transfer

• Transferring Data to PC

Connect the instrument to a PC and Data Acquisition Software (DAS) using the phono to USB cable to transfer stored data.

1. Connect the phono jack of the cable to the back of the instrument and the USB connector to the communication port of the PC.
2. Install the DAS in the PC and follow the procedures in the DAS instruction sheet.

• Printing Data

Connect the instrument to a printer using the phono to 25-pin d-sub printer cable and follow the procedure below to print a data set.

1. In measurement mode, press  key.
2. Use   keys to view stored data.
3. Press  key to print the selected data.

• Printer Format - Stored Data

Model	PC2000
S/No	A81J1234
SW Rev	1.00
User Name	
Signature	
Logged Data	
Location	13
Date	23APR2021
Time	09:41:48
Mode	pH
Stability	STABLE
pH	4.03 pH
mV	162.3 mV
Temp.	23.8 C (ATC)
Electrode	EXCELLENT

Tip

To print entire stored data log, refer "Print Data Log Setup" on page 54.

■ Setup

This section describes the setups in Environmental Express Series 2000 benchtop meters.

● P1 pH Setup

Using pH setup you can:

- Set pH buffer group
- Set pH resolution
- Set calibration alarm
- Erase calibration data

To set the pH function of Environmental Express PH2000, ION2000, or PC2000 meter, follow the procedure detailed below:

Prerequisites

- Switch on the meter.
- Ensure that the meter is in pH measurement mode.

Note

- Default pH buffer group in buffer setup is **USA**. You can change it to **NIST**, **NIST2**, **DIN**, or **CUST** (Custom) if required.
- Erasing previous calibration data is recommended for accurate calibration. Default calibration clear setup is **NO** but to erase the calibration data, change the setup to **YES**.


pH Buffer Group	pH Buffer Values (25°C)
USA	1.68, 4.01, 7.00, 10.01, 12.45
NIST	1.68, 4.01, 6.86, 9.18, 12.45
NIST2	1.68, 4.01, 6.86, 10.01, 12.45
DIN	1.09, 3.06, 4.65, 6.79, 9.23, 12.75
CUST	Use up to 6 pH buffers that are 1.0 pH apart for manual calibration

Tip

To return to the measurement mode, press the  key.


• P1.1 Buffer Setup

1. Press the  key, **P1 PH** screen appears.
2. Press the **ENT**  key, **P1.1 BUFF** screen appears.
3. Press the **ENT**  key, default **buff USA** appears.
4. Use the   keys to change the pH buffer group to **NIST**, **NIST2**, **DIN** or **CUST**.
5. Press the **ENT**  key, **P1.1 BUFF** screen appears. This indicates completion of pH buffer group setup.

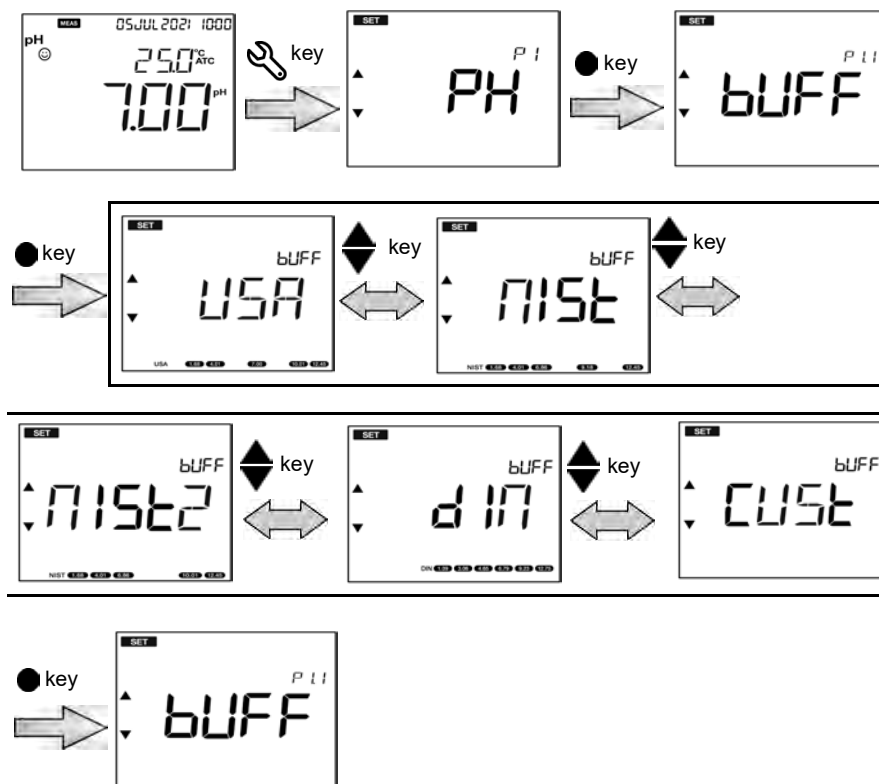


• P1.2 Resolution Setup

1. Press the  key, **P1 PH** screen appears.
2. Press the **ENT**  key, **P1.1 BUFF** screen appears.
3. Press the  key, **P1.2 RESOL** screen appears.
4. Press the **ENT**  key, default resolution **0.001** screen appears.
5. Use the   keys to change the resolution to **0.01** or **0.1**.
6. Press the **ENT**  key, **P1.2 RESOL** screen appears. This indicates completion of resolution setup.

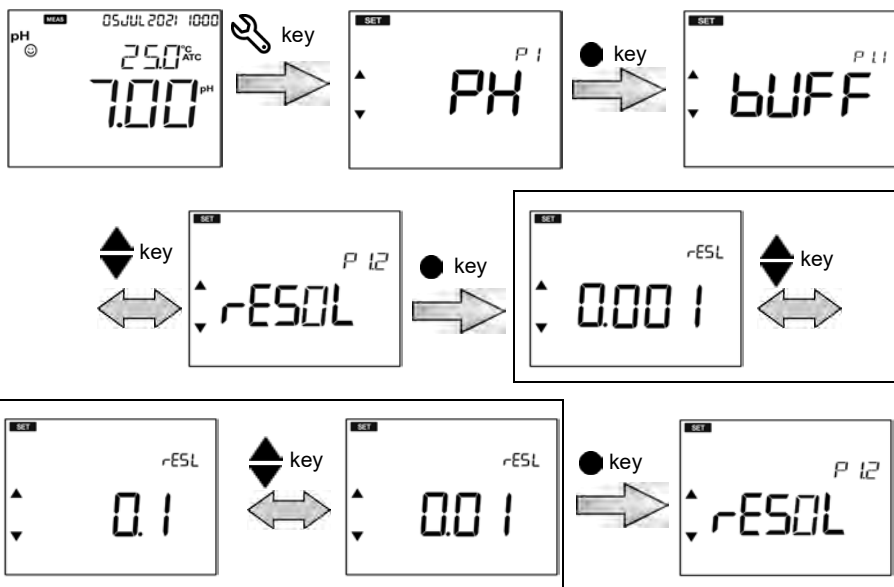


• P1.3 Calibration Alarm Setup

1. Press the  key, **P1 PH** screen appears.
2. Press the **ENT**  key, **P1.1 BUFF** screen appears.
3. Press the  key, **P1.2 RESOL** screen appears.
4. Press the  key, **P1.3 C.ALr** screen appears.
5. Press the **ENT**  key, default ---- **DAYS** screen appears.
6. Use the   and   keys to set number of days from 1 to 90.
7. Press the **ENT**  key, **P1.3 C.ALr** screen appears. This indicates completion of calibration alarm setup.

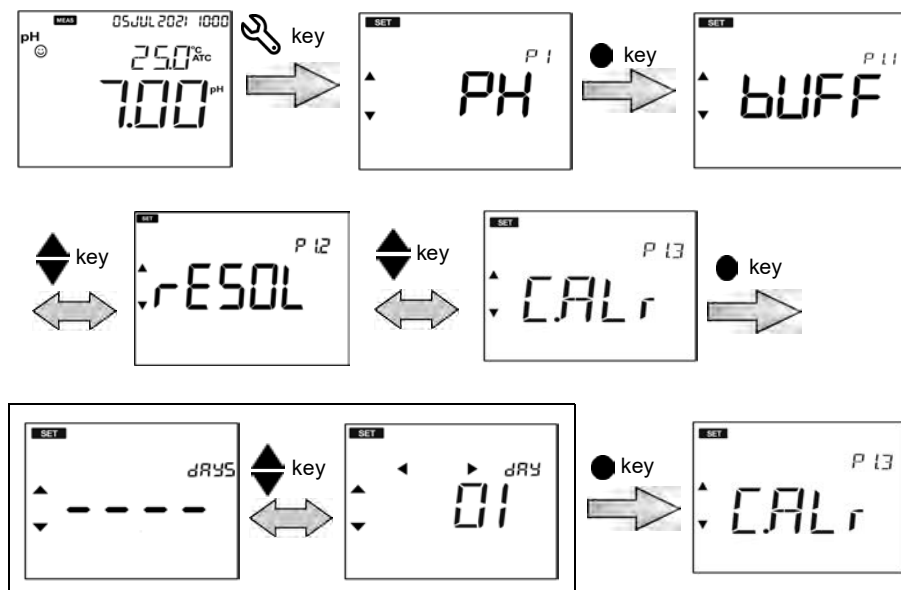

• P1.4 Calibration Clear Setup

1. Press the  key, **P1 PH** screen appears.
2. Press the **ENT**  key, **P1.1 BUFF** screen appears.
3. Press the  key, **P1.2 RESOL** screen appears.
4. Press the  key, **P1.3 C.ALK** screen appears.
5. Press the  key, **P1.4 C.CLR** screen appears.
6. Press the **ENT**  key, default **CCLR NO** screen appears.
7. Use the   keys to change to **YES**. This erases the calibration data.
8. Press the **ENT**  key, **CCLR DONE** screen appears briefly.
9. **P1.4 C.CLR** screen appears. This indicates completion of calibration clear setup.

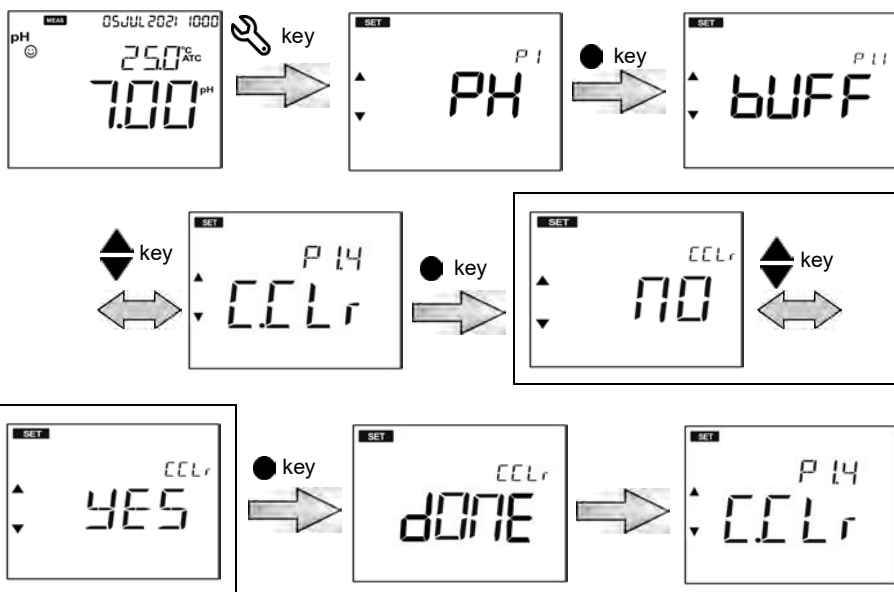

• P1 Ion Setup

Using ion setup you can:

- Select ion concentration unit
- Select ion electrode type or set the valence of the ion to be measured
- Erase calibration data

To set the ion function of Environmental Express ION2000 or PC2000 meter, follow the procedure detailed below:

Prerequisites




- Switch on the meter.
- Ensure that the meter is in ion measurement mode.

Note

- Default ion concentration unit is $\mu\text{g/L} \leftrightarrow \text{mg/L} \leftrightarrow \text{g/L}$. You can change it to $\text{ppm} \leftrightarrow \text{ppt}$ or $\text{mmol/L} \leftrightarrow \text{mol/L}$, if required.
- Default ion electrode type is **NH3** (Ammonia). You can change it to **CL** (Chloride), **FL** (Fluoride), **NO3** (Nitrate), **POT** (Potassium), **CA** (Calcium) or **CUST** (Custom). **CUST** is for setting the valence of the ion to be measured when the ion electrode type in use is not in the selection.
- Erasing previous calibration data is recommended for accurate calibration. Default calibration clear setup is **NO** but to erase the calibration data, change the setup to **YES**.


● P1.1 Ion Concentration Unit Setup


1. Press the  key, **P1 ION** screen appears.
2. Press the **ENT**  key, **P1.1 UNIT** screen appears.
3. Press the **ENT**  key, default **µg/L ↔ mg/L ↔ g/L** appears.
4. Use the   keys to change the ion concentration unit to **ppm ↔ ppt** or **mmol/L ↔ mol/L**.
5. Press the **ENT**  key, **P1.1 UNIT** screen appears. This indicates completion of ion concentration unit setup.

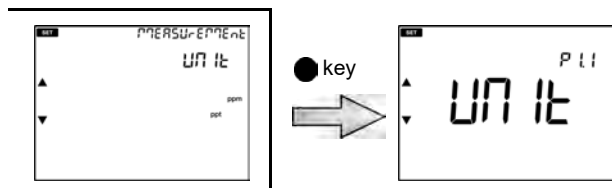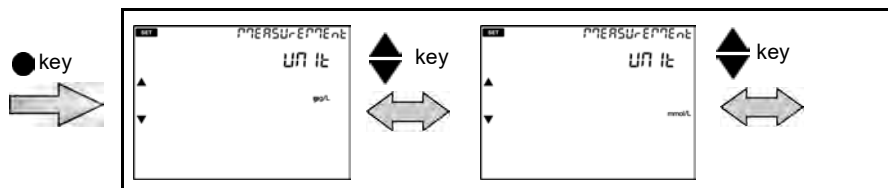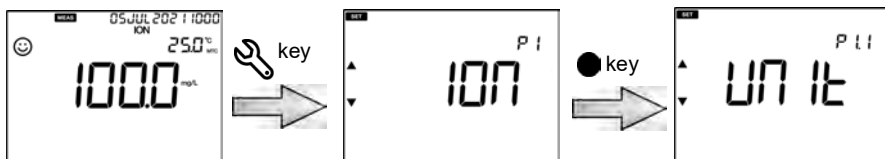

• P1.2 Ion Electrode Type Setup


1. Press the  key, **P1 ION** screen appears.
2. Press the **ENT**  key, **P1.1 UNIT** screen appears.
3. Press the  key, **P1.2 TYPE** screen appears.
4. Press the **ENT**  key, default **NH3** (Ammonia) ion electrode type appears.
5. Use the   keys to change the electrode type to **CA** (Calcium), **POT** (Potassium), **NO3** (Nitrate), **FL** (Fluoride), **CL** (Chloride), or **CUST** (Custom). If **CUST** is selected, default **CHRG 1** screen appears after pressing **ENT**  key. Use   keys to change to **-1**, **2**, or **-2** depending on the valence of the ion to be measured.
6. Press the **ENT**  key, **P1.2 TYPE** screen appears indicating completion of ion electrode type setup.

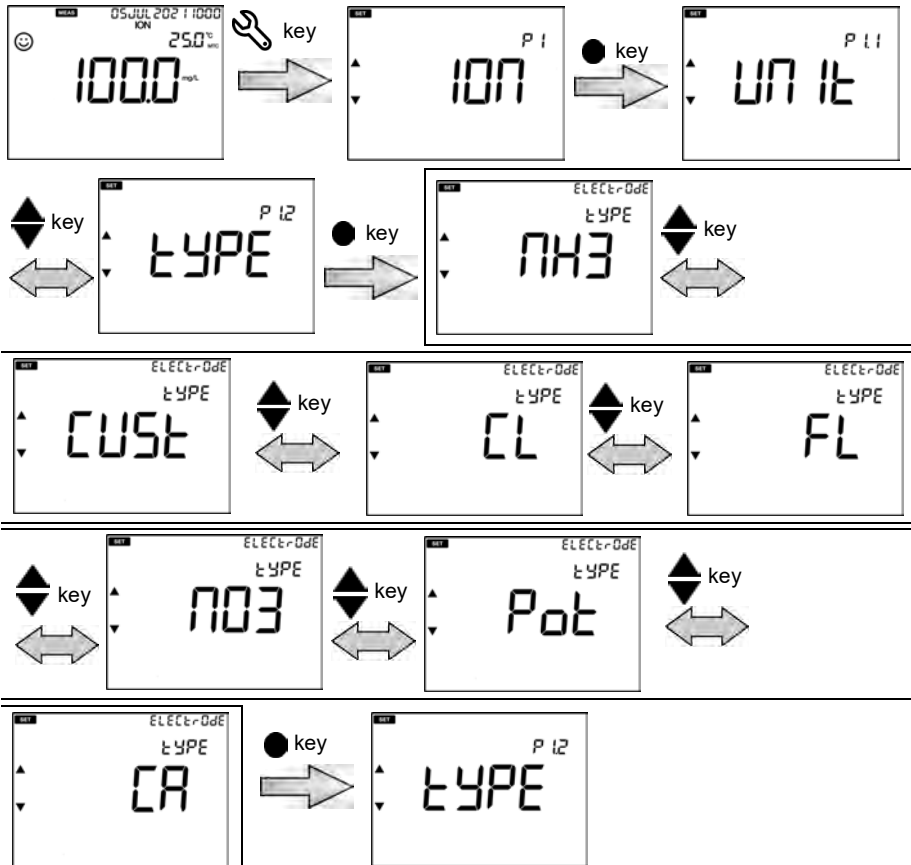

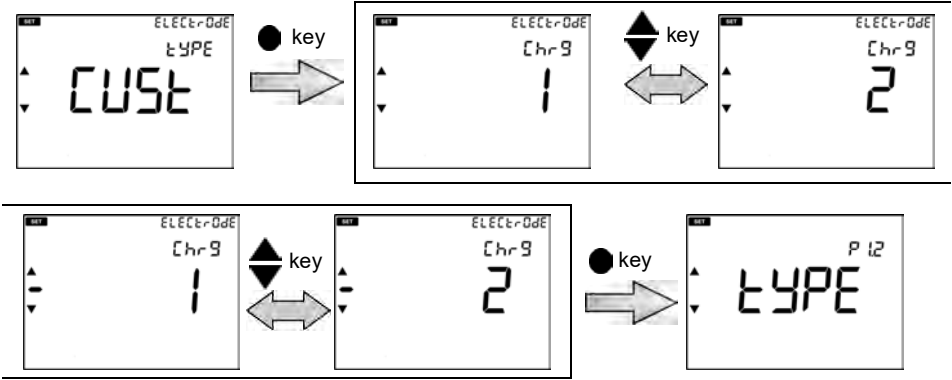

• P1.3 Calibration Clear Setup

1. Press the  key, **P1 ION** screen appears.
2. Press the **ENT**  key, **P1.1 UNIT** screen appears.
3. Press the  key, **P1.2 TYPE** screen appears.
4. Press the  key, **P1.3 C.CLR** screen appears.
5. Press the **ENT**  key, default **CCLR NO** screen appears.
6. Use the   keys to change to **YES**. This erases the ion calibration data.
7. Press the **ENT**  key, **CCLR DONE** screen appears briefly.
8. **P1.3 C.CLR** screen appears. This indicates completion of calibration clear setup.

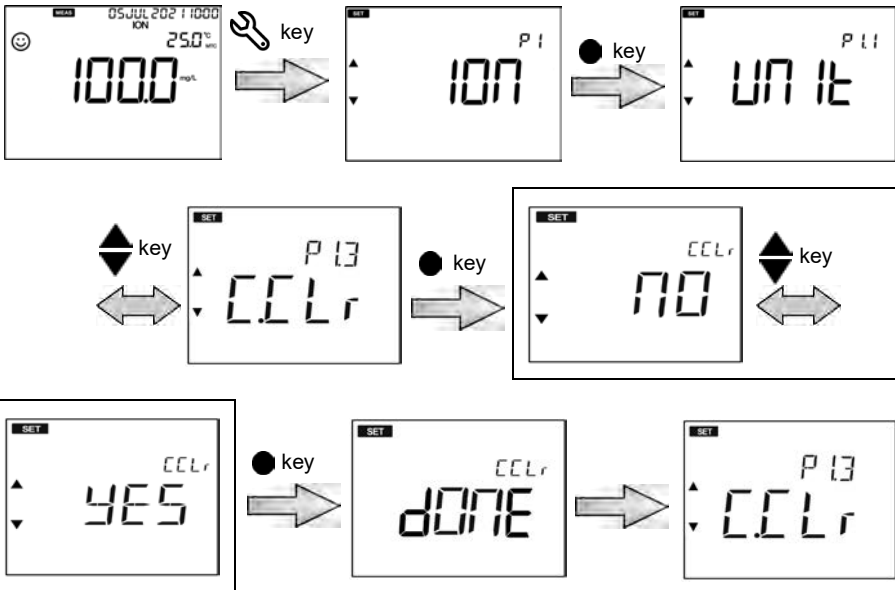

• P1 COND Setup

Using conductivity setup, you can:

- Set cell constant
- Select conductivity unit
- Select calibration method
- Set temperature coefficient
- Set reference temperature
- Erase calibration data

To set the conductivity function of Environmental Express EC2000 or PC2000 meter, follow the procedure detailed below:

Prerequisites

- Switch on the meter.
- Ensure that the meter is in conductivity measurement mode.

Note

- Default cell constant value is **1.0000**. You can set a value in between **0.0700 to 13.000**.
 - Default conductivity unit is **S/cm**. You can change the unit to **S/m**.
 - Default auto calibration setup is **ON**. To perform manual calibration, change the setup to **OFF**.
 - Default temperature coefficient is **2.00%**. You can set a value in between **00.00% to 10.00%**.
 - Default reference temperature is **25.0°C**. You can set the value in between **15.0°C to 30.0°C**.
 - Erasing previous calibration data is recommended for accurate calibration. Default calibration clear setup is **NO** but to erase the calibration data, change the setup to **YES**.
-

Tip


To return to the measurement mode, press the  key.

● P1.1 Cell Constant Setup

1. Press the  key, **P1 COND** screen appears.
2. Press the **ENT**  key, **P1.1 CELL** screen appears.
3. Press the **ENT**  key, default **CELL 1.0000** appears.
4. Use the   and   keys to set the cell constant in between 0.0700 to 13.000.


Use the  key to move the decimal point.

5. Press the **ENT**  key, **P1.1 CELL** screen appears. This indicates completion of cell constant setup.

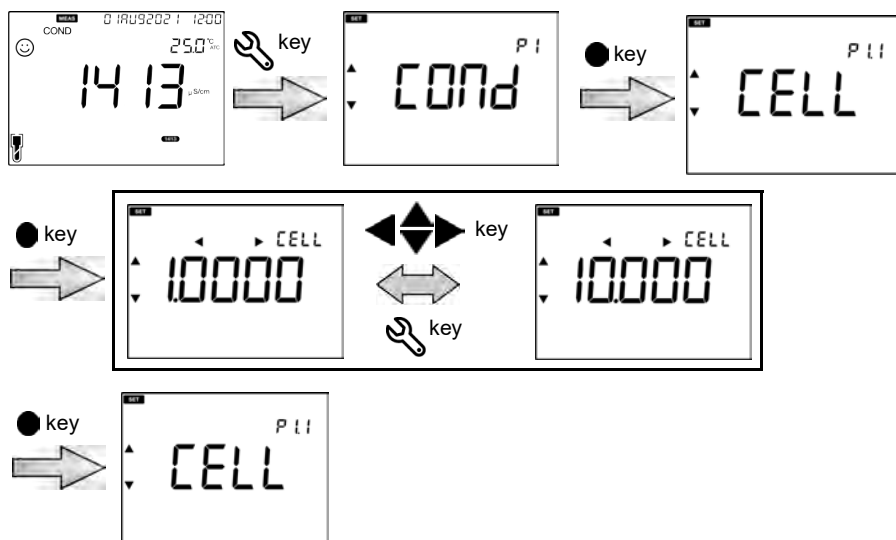


• P1.2 Conductivity Unit Setup

1. Press the  key, **P1 COND** screen appears.
2. Press the **ENT**  key, **P1.1 CELL** screen appears.
3. Press the  key, **P1.2 UNIT** screen appears.
4. Press the **ENT**  key, default **UNIT S/cm** appears.
5. Use the   keys to change the conductivity unit to **S/m**.
6. Press the **ENT**  key, **P1.2 UNIT** screen appears. This indicates completion of conductivity unit setup.

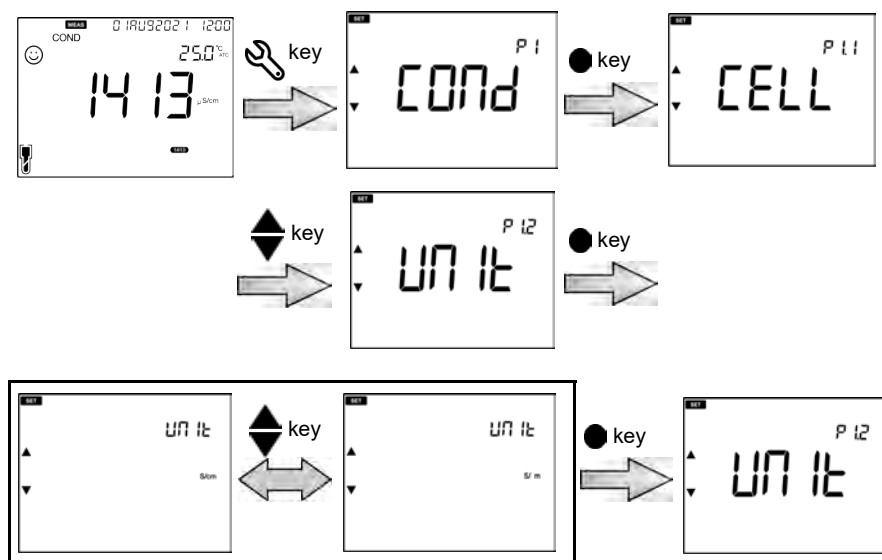


• P1.3 Auto Calibration Setup

1. Press the  key, **P1 COND** screen appears.
2. Press the **ENT**  key, **P1.1 CELL** screen appears.
3. Press the  key, **P1.2 UNIT** screen appears.
4. Press the  key, **P1.3 A.CAL** appears.
5. Press the **ENT**  key, default **A.CAL ON** screen appears.
6. Use the   keys to change to **OFF**. This enables the manual calibration method.
7. Press the **ENT**  key, **P1.3 A.CAL** screen appears. This indicates completion of auto calibration setup.

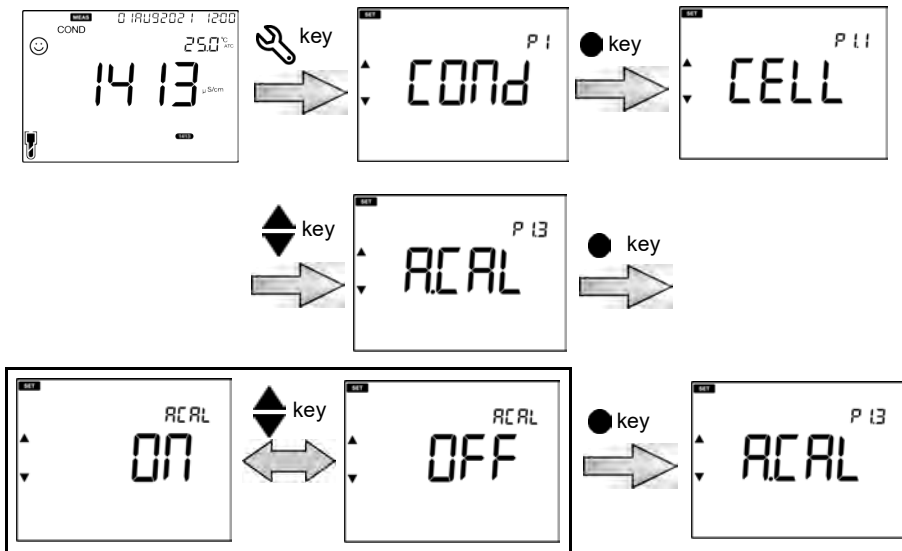


• P1.4 Temperature Coefficient Setup

1. Press the  key, **P1 COND** screen appears.
2. Press the **ENT**  key, **P1.1 CELL** screen appears.
3. Press the  key, **P1.2 UNIT** screen appears.
4. Press the  key, **P1.3 A.CAL** appears.
5. Press the  key, **P1.4 T.CFF** appears.
6. Press the **ENT**  key, default **2.00%** appears.
7. Use the   keys to set the temperature coefficient in between 00.00% to 10.00%.
8. Press the **ENT**  key, **P1.4 T.CFF** screen appears. This indicates completion of temperature coefficient setup.

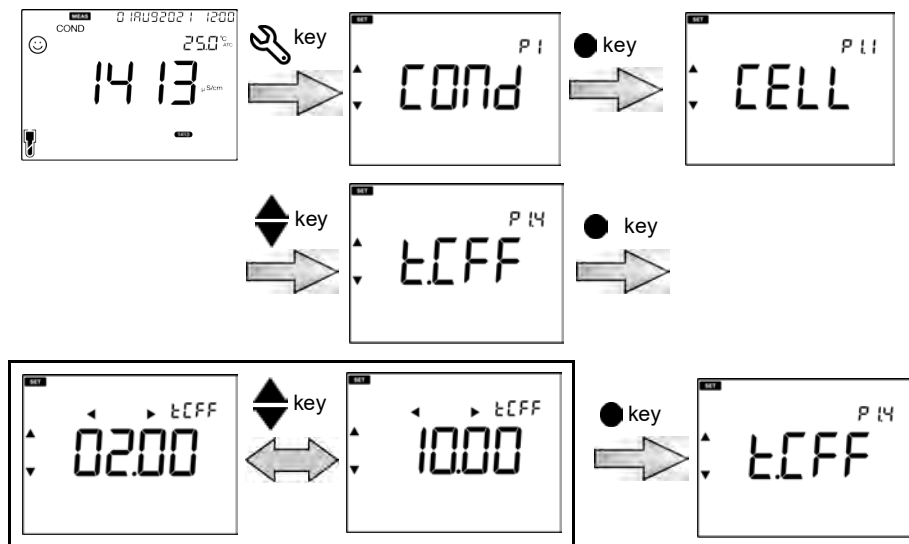


• P1.5 Reference Temperature Setup

1. Press the  key, **P1 COND** screen appears.
2. Press the **ENT**  key, **P1.1 CELL** screen appears.
3. Press the  key, **P1.2 UNIT** screen appears.
4. Press the  key, **P1.3 A.CAL** appears.
5. Press the  key, **P1.4 T.CFF** appears.
6. Press the  key, **P1.5 T.REF** appears.
7. Press the **ENT**  key, default **25.0°C** appears.
8. Use the   keys to set the reference temperature in between 15.0°C to 30.0°C.
9. Press the **ENT**  key, **P1.5 T.REF** screen appears. This indicates completion of reference temperature setup.

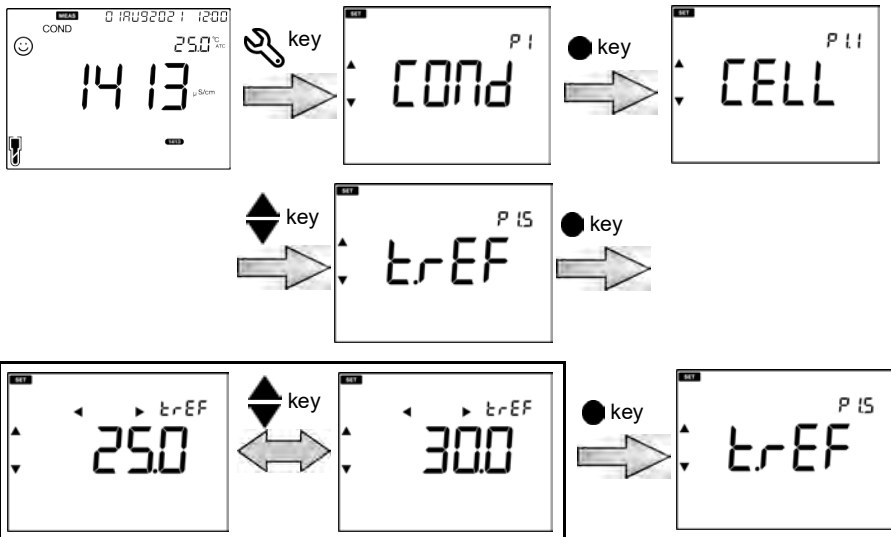

• P1.6 Calibration Clear Setup

1. Press the  key, **P1 COND** screen appears.
2. Press the **ENT**  key, **P1.1 CELL** screen appears.
3. Press the  key, **P1.2 UNIT** screen appears.
4. Press the  key, **P1.3 A.CAL** appears.
5. Press the  key, **P1.4 T.CFF** appears.
6. Press the  key, **P1.5 T.REF** appears.
7. Press the  key, **P1.6 C.CLR** appears.
8. Press the **ENT**  key, default **NO** screen appears.
9. Use the   keys to change to **YES**. This erases the calibration data.
10. Press the **ENT**  key, **CCLR DONE** screen appears briefly.
11. **P1.6 C.CLR** screen appears. This indicates completion of calibration clear setup.

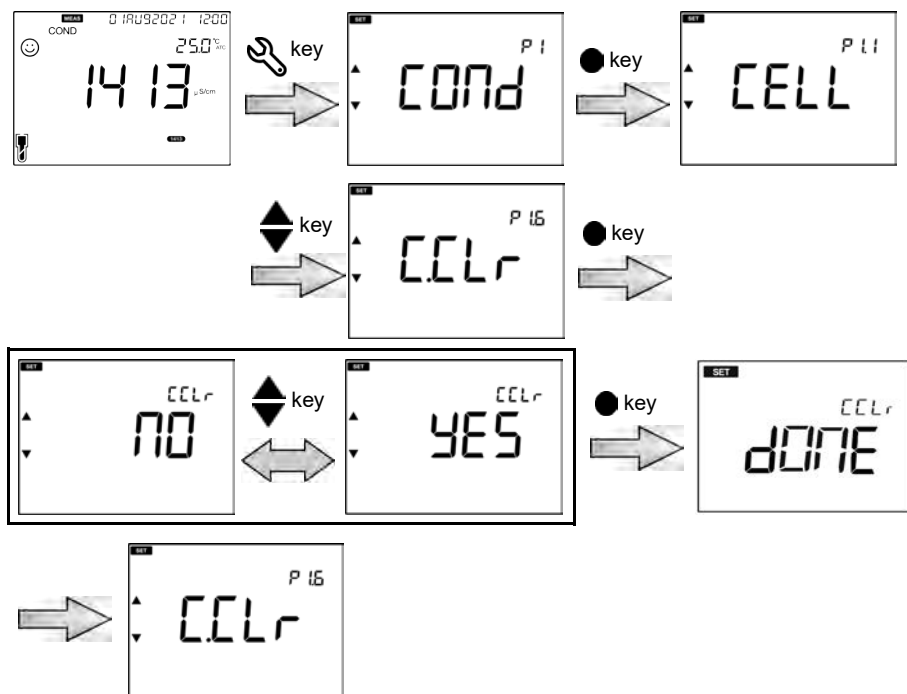

• P2 TDS Setup

Using TDS setup, you can:

- Select TDS curve
- Select TDS unit

To set the TDS function of Environmental Express EC2000 or PC2000 meter, follow the procedure detailed below:

Prerequisites

- Switch on the meter.
- Ensure that the meter is in TDS measurement mode.

Note


- Default TDS curve is **LINR** (Linear). You can change the TDS curve to **442** or **EN** (EN27888) or **NACL** (NaCl).
- For **LINR** curve, default multiplier factor is **FACT 0.50**. You can set a multiplier factor in between **0.40** to **1.00**.
- Default TDS unit is **mg/L** ↔ **g/L** . You can change the unit to **ppm** ↔ **ppt**.

Tip


To return to the measurement mode, press the  key.

• P2.1 TDS Curve Setup

- 1. Press the  key, **P1 COND** screen appears.
- 2. Press the  key, **P2 TDS** screen appears
- 3. Press the **ENT**  key, **P2.1 FACT** screen appears.
- 4. Press the **ENT**  key, default **FACT LINr** appears.
- 5. Use the   keys to select a TDS curve. If **LINr** is desired, press **ENT**  key to select and use   and   keys to set a factor in between 0.40 to 1.00 (default 0.50).
- 6. Press the **ENT**  key, **P2.1 FACT** screen appears. This indicates completion of TDS curve setup.

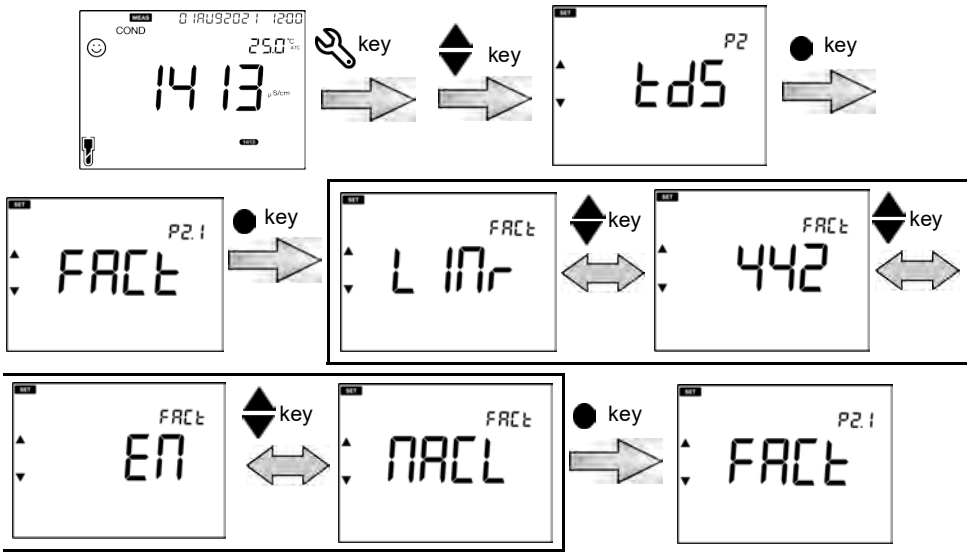


If you choose **LINr**, you can set a factor in between **0.40 to 1.00**.

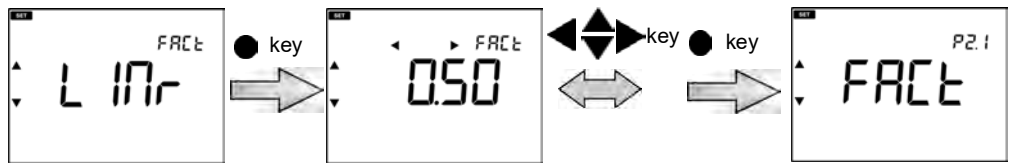

• P2.2 TDS Unit Setup

1. Press the  key, **P1 COND** screen appears.
2. Press the  key, **P2 TDS** screen appears.
3. Press the **ENT**  key, **P2.1 FACT** screen appears.
4. Press the  key, **P2.2 UNIT** screen appears.
5. Press the **ENT**  key, default **UNIT mg/L ↔ g/L** screen appears
6. Use the   keys to change the TDS unit to **ppm ↔ ppt**.
7. Press the **ENT**  key, **P2.2 UNIT** screen appears. This indicates completion of TDS unit setup.

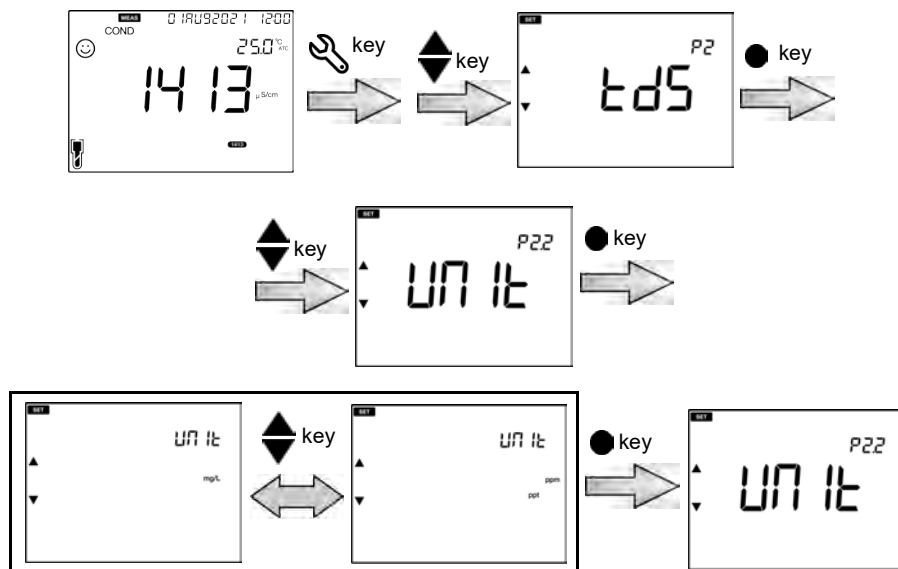

● P3 SAL Setup

Using salinity setup, you can:

- Select salinity unit
- Select salinity type
- Erase calibration data

To set the salinity function of Environmental Express EC2000 or PC2000 meter, follow the procedure detailed below:

Prerequisites

- Switch on the meter.
- Ensure that the meter is in salinity measurement mode.

Note


- Default salinity unit is **ppt** (parts per thousand). You can change the unit to **%** (percentage).
 - Default salinity type is **NACL** (NaCl). You can change the salinity type to **SEA.W** (seawater).
 - Erasing previous calibration data is recommended for accurate calibration. Default calibration clear setup is **NO** but to erase the calibration data, change the setup to **YES**.
-

Tip

To return to the measurement mode, press the  key.




• P3.1 Salinity Unit Setup

1. Press the  key, **P1 COND** screen appears.
2. Press the  key, **P2 TDS** screen appears.
3. Press the  key, **P3 SAL** screen appears.
4. Press the **ENT**  key, **P3.1 UNIT** screen appears.
5. Press the **ENT**  key, default **UNIT ppt** appears.
6. Use the   keys to change the salinity unit to %.
7. Press the **ENT**  key, **P3.1 UNIT** screen appears. This indicates completion of salinity unit setup.

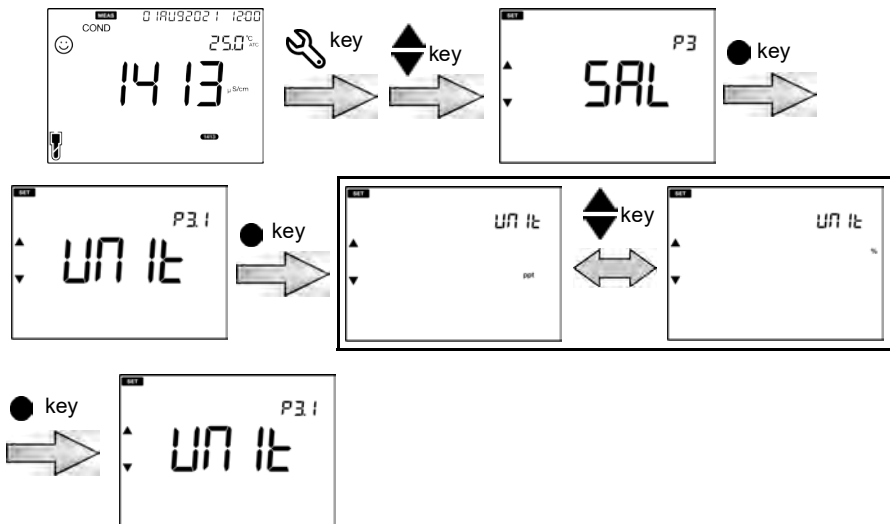


● **P3.2 Salinity Type Setup**

- 1. Press the  key, **P1 COND** screen appears.
- 2. Press the  key, **P2 TDS** screen appears.
- 3. Press the  key, **P3 SAL** screen appears.
- 4. Press the **ENT**  key, **P3.1 UNIT** screen appears.
- 5. Press the  key, **P3.2 TYPE** screen appears.
- 6. Press the **ENT**  key, default **TYPE NA_{CL}** (NaCl) appears.
- 7. Use the   keys to change the salinity type to **SEA.W** (seawater).
- 8. Press the **ENT**  key, **P3.2 TYPE** screen appears. This indicates completion of salinity type setup.

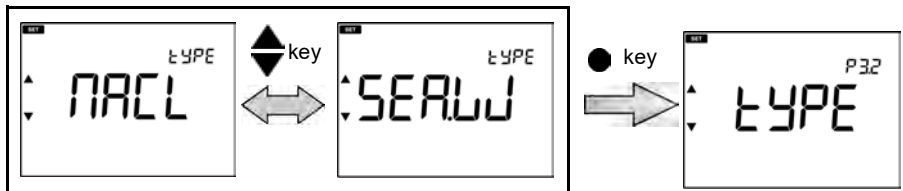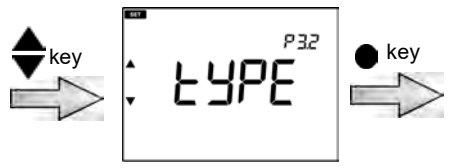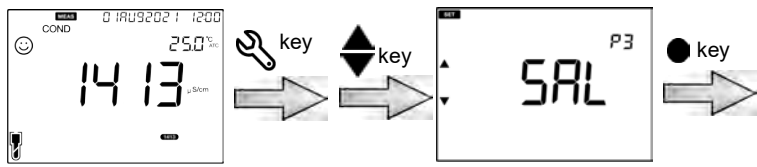

● P3.3 Calibration Clear Setup

1. Press the  key, **P1 COND** screen appears.
2. Press the  key, **P2 TDS** screen appears.
3. Press the  key, **P3 SAL** screen appears.
4. Press the **ENT**  key, **P3.1 UNIT** screen appears.
5. Press the  key, **P3.2 TYPE** screen appears.
6. Press the  key, **P3.3 C.CLR** screen appears.
7. Press the **ENT**  key, default **C.CLR NO** appears.
8. Use the   keys to change to **YES**. This erases the calibration data.
9. Press the **ENT**  key, **CCLR DONE** screen appears briefly.
10. **P3.3 C.CLR** screen appears. This indicates completion of calibration clear setup.

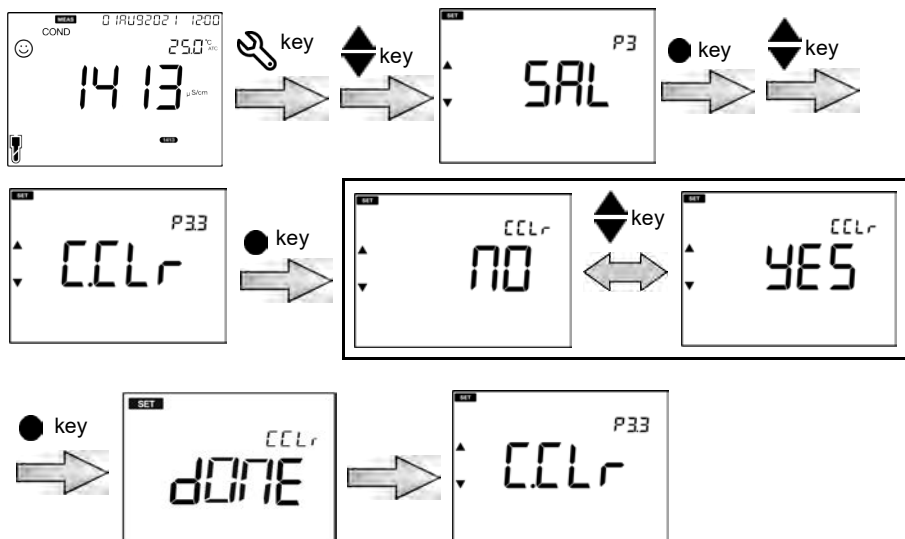

• Data Setup

Using data setup, you can:

- Set data log interval
- Print data log
- Erase data log

To set the data function, follow the procedure detailed below:

Prerequisites

- Switch on the meter.
- Keep the meter in either pH or ion or conductivity mode.

Note


- Default data log interval is “----” which indicates no data log interval has been set. Data log interval can be set from 2 to 999 seconds.
-

Tip

To return to the measurement mode, press the  key.

• Data Log Interval Setup

1. Press the  key, **P1 PH / ION / COND** screen appears.
2. Press the  key, **P2 / P4 DATA** screen appears.
3. Press the **ENT**  key, **P2.1 / P4.1 LOG** screen appears.
4. Press the **ENT**  key, default ---- log interval appears.
5. Use the   and   keys to set the data log interval from 2 to 999 seconds.
6. Press the **ENT**  key, **P2.1 / P4.1 LOG** screen appears. This indicates completion of data log interval setup.

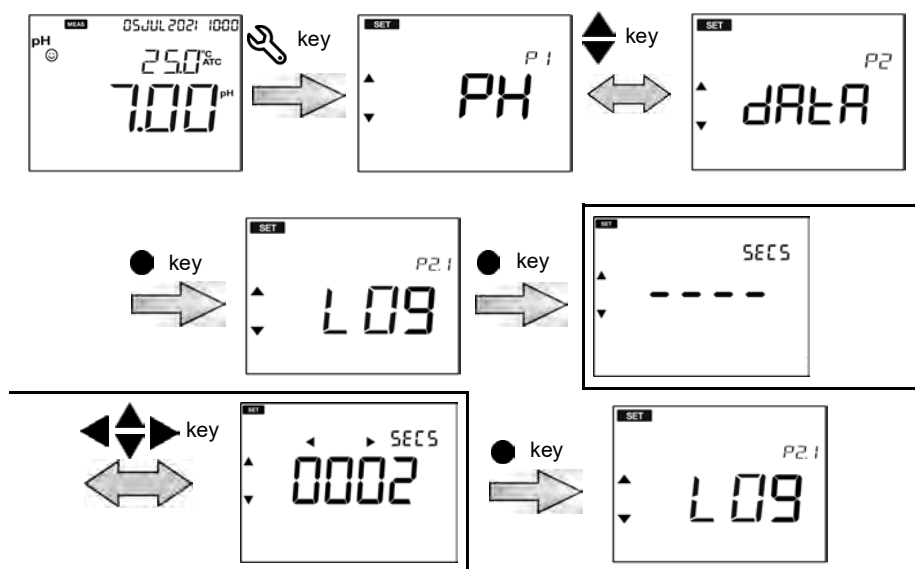


Tip

To start and stop auto data logging in measurement mode, press  key.

• Print Data Log Setup

1. Press the  key, **P1 PH / ION / COND** screen appears.
2. Press the  key, **P2 / P4 DATA** screen appears.
3. Press the **ENT**  key, **P2.1 / P4.1 LOG** screen appears.
4. Press the  key, **P2.2 / P4.2 PRINT** screen appears.
5. Press the **ENT**  key, default **NO** appears.
6. Use the   keys to change to **YES**. This prints all stored data.
7. Press the **ENT**  key, **LOC END** screen appears briefly after the last data is printed.
8. **P2.2 / P4.2 PRINT** screen appears. This indicates the completion of the print data log setup.

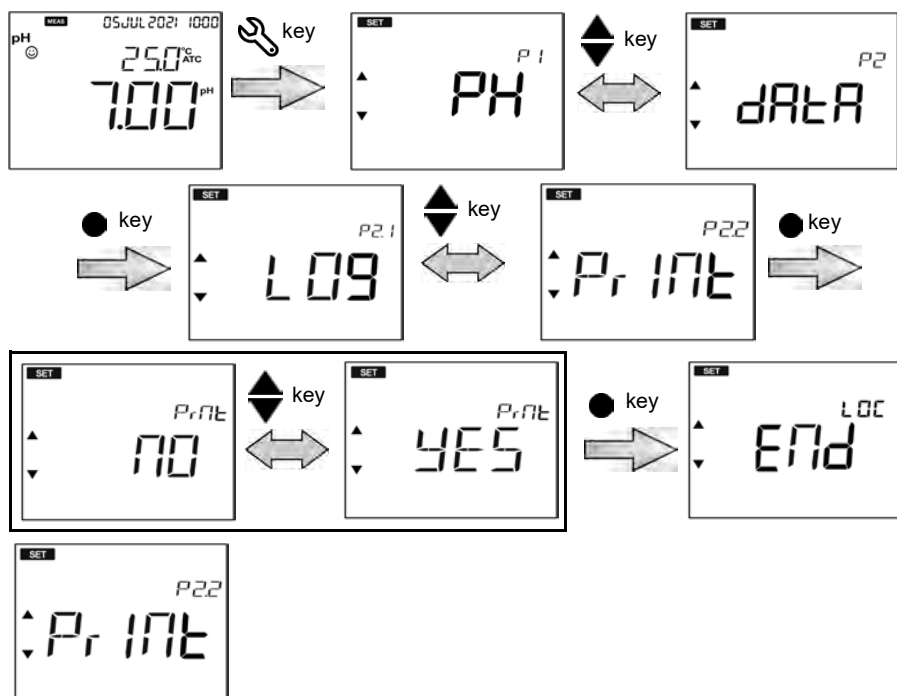


Tip

To stop the printing process, press and hold the  key.

• Data Log Clear Setup

1. Press the  key, **P1 PH / ION / COND** screen appears.
2. Press  key, **P2 / P4 DATA** screen appears.
3. Press the **ENT**  key, **P2.1 / P4.1 LOG** screen appears.
4. Press the  key, **P2.2 / P4.2 PRINT** screen appears.
5. Press the  key, **P2.3 / P4.3 D.CLR** screen appears.
6. Press the **ENT**  key, default **NO** appears
7. Use the   keys to change to **YES**. This erases all data.
8. Press the **ENT**  key, **D.CLR DONE** screen appears briefly.
9. **P2.3 / P4.3 D.CLR** screen appears. This indicates the completion of data log clear setup.

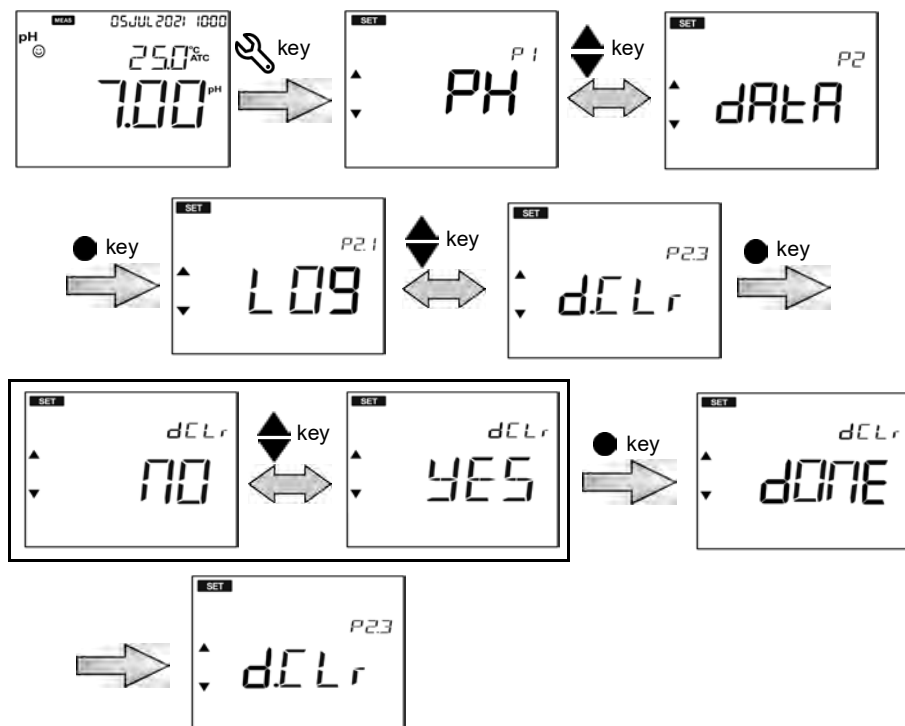

• General Setup

Using general setup, you can:

- Set reading stability mode
- Set auto shut-off time
- Set temperature unit
- Set password for setup mode
- Reset the meter

To set the general function, follow the procedure detailed below:

Prerequisites

- Switch on the meter.
- Keep the meter in either pH or ion or conductivity mode.

Note

- In calibration mode, the Auto Stable (**AS**) mode is activated. Default reading stability mode setup in measurement mode is Auto Stable (**AS**). You can change it to Auto Hold (**AH**) or Real Time (**RT**).
 - Default auto shut-off time is 30 minutes. You can set the time from ---- to 30 minutes, where ---- indicates “no auto shut-off time” has been set and meter will be “on” continuously.
 - Default temperature unit is °C and you can change it to °F.
 - Default reset meter setup is **NO**. You can change it to **YES**.
-

Tip

- Stability judgment criteria remains same for both Auto Stable mode and Auto Hold mode.
 - To return to the measurement mode, press the  key.
-




• Reading Stability Mode Setup

Auto Stable (AS) Mode – The meter shows live readings; 😊 blinks until reading is stable.

Auto Hold (AH) Mode – The meter locks the stable reading; 😊 blinks until reading is stable and then **HOLD** lights up.


Real Time (RT) Mode – The meter shows live readings; both 😊 and **HOLD** are inactive.

1. Press the  key, **P1 PH / ION / COND** screen appears.
2. Press  key, **P2 / P4 DATA** screen appears.
3. Press  key, **P3 / P5 GEN** screen appears.
4. Press the **ENT**  key, **P3.1 / P5.1 STBLE** screen appears.
5. Press the **ENT**  key, the default **AS** (Auto Stable) reading stability mode appears.
6. Use the   keys to change to **AH** (Auto Hold) or **RT** (Real Time).
7. Press the **ENT**  key, **P3.1 / P5.1 STBLE** screen appears. This indicates completion of the reading stability mode setup.

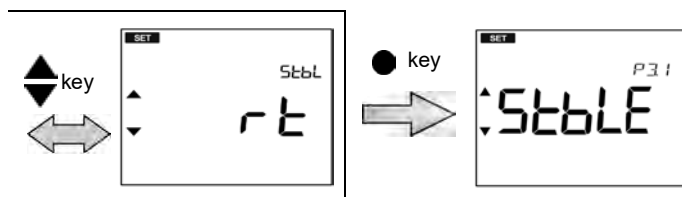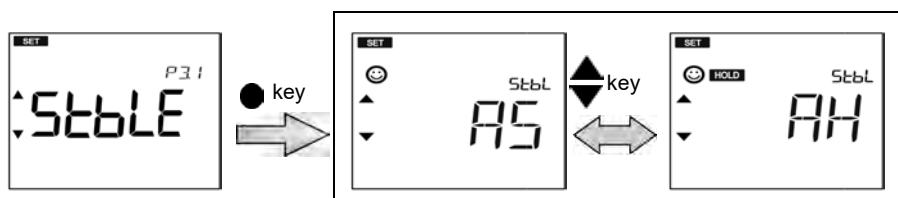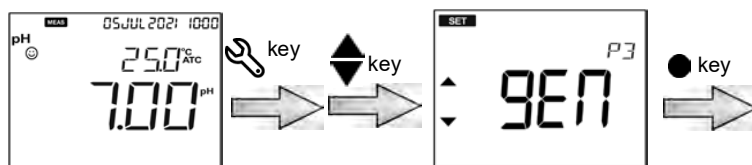


● Auto Shut-off Time Setup

1. Press the  key, **P1 PH / ION / COND** screen appears.
2. Press the  key, **P2 / P4 DATA** screen appears.
3. Press the  key, **P3 / P5 GEN** screen appears.
4. Press the **ENT**  key, **P3.1 / P5.1 STBLE** screen appears.
5. Press the  key, **P3.2 / P5.2 A.OFF** screen appears.
6. Press the **ENT**  key, default auto shut-off time **30 minutes** appear.
7. Use the   and   keys to adjust the auto shut-off time from ---- to 30 minutes.
8. Press the **ENT**  key, **P3.2 / P5.2 A.OFF** screen appears. This indicates completion of the auto shut-off time setup.

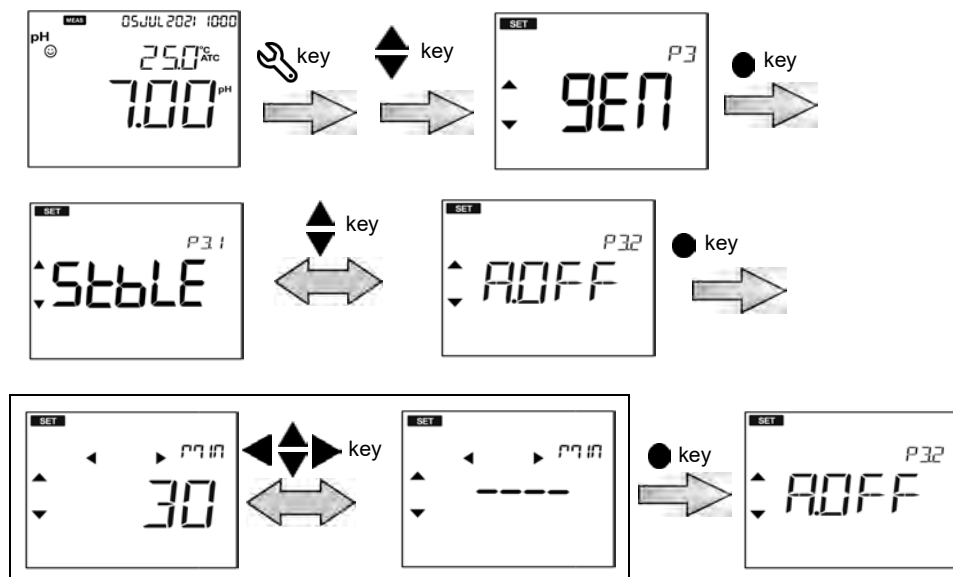


• Temperature Unit Setup

1. Press the  key, **P1 PH / ION / COND** screen appears.
2. Press the  key, **P2 / P4 DATA** screen appears.
3. Press the  key, **P3 / P5 GEN** screen appears.
4. Press the  key, **P3.1 / P5.1 STBLE** screen appears.
5. Press the  key, **P3.2 / P5.2 A.OFF** screen appears.
6. Press the  key, **P3.3 / P5.3 °C°F** screen appears.
7. Press the **ENT**  key, default temperature unit °C appears.
8. Use the   keys to change to °F.
9. Press the **ENT**  key, **P3.3 / P5.3 °C°F** screen appears. This indicates completion of the temperature unit setup.

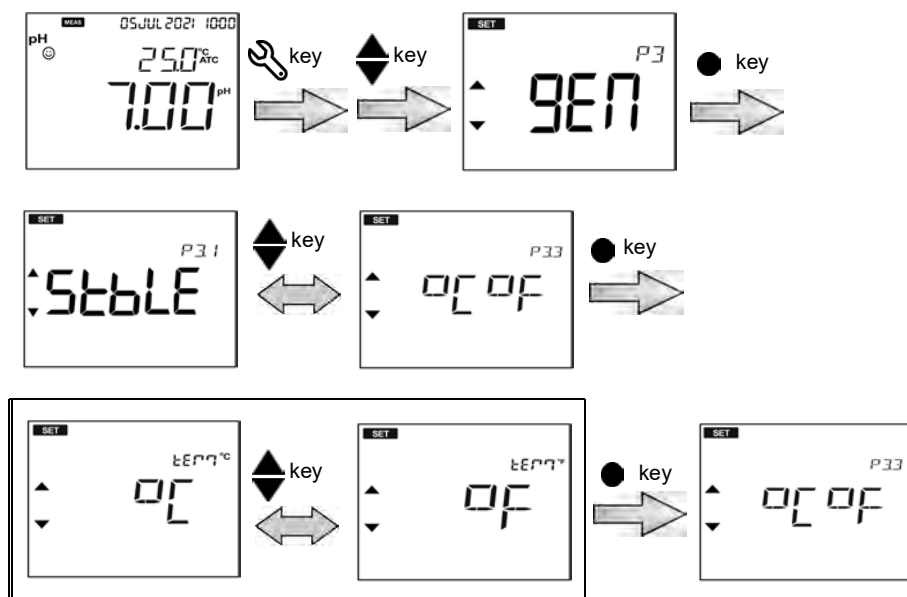


• Password Setup

1. Press the  key, **P1 PH / ION / COND** screen appears.
2. Press the  key, **P2 / P4 DATA** screen appears.
3. Press the  key, **P3 / P5 GEN** screen appears.
4. Press the **ENT**  key, **P3.1 / P5.1 STBLE** screen appears.
5. Press the  key, **P3.2 / P5.2 A.OFF** screen appears.
6. Press the  key, **P3.3 / P5.3 °C°F** screen appears.
7. Press the  key, **P3.4 / P5.4 PASS** screen appears.
8. Press the **ENT**  key, default **PASS OFF** appears.
9. Press the  key, **PASS ON** screen appears. This restricts access to setup mode.
10. Press the  key. Use the   and   keys to set password up to 4 digits.
11. Press the  key, **P3.4 / P5.4 PASS** screen appears. This indicates completion of the password setup.

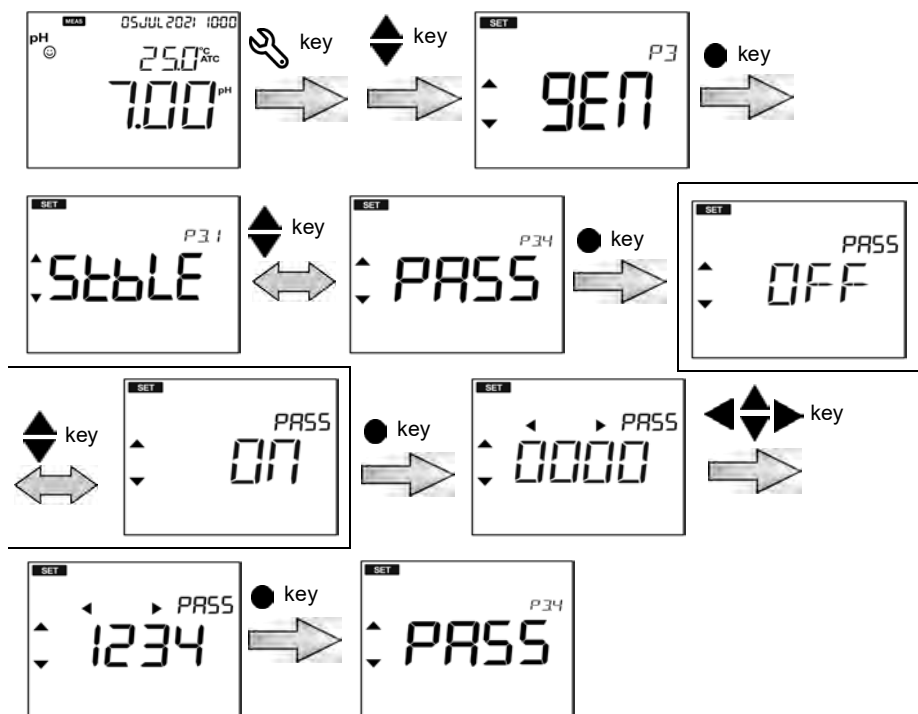

• Reset Setup

1. Press the  key, **P1 PH / ION / COND** screen appears.
2. Press the  key, **P2 / P4 DATA** screen appears.
3. Press the  key, **P3 / P5 GEN** screen appears.
4. Press the **ENT**  key, **P3.1 / P5.1 STBLE** screen appears.
5. Press the  key, **P3.2 / P5.2 A.OFF** screen appears.
6. Press the  key, **P3.3 / P5.3 °C°F** screen appears.
7. Press the  key, **P3.4 / P5.4 PASS** screen appears.
8. Press the  key, **P3.5 / P5.5 RESET** screen appears.
9. Press the **ENT**  key, default reset **NO** appears.
10. Use the   keys to change to **YES**. This resets the meter to factory default values.
11. Press the  key, meter displays **RESET DONE** and then **RESET END** briefly, before it automatically switches off.

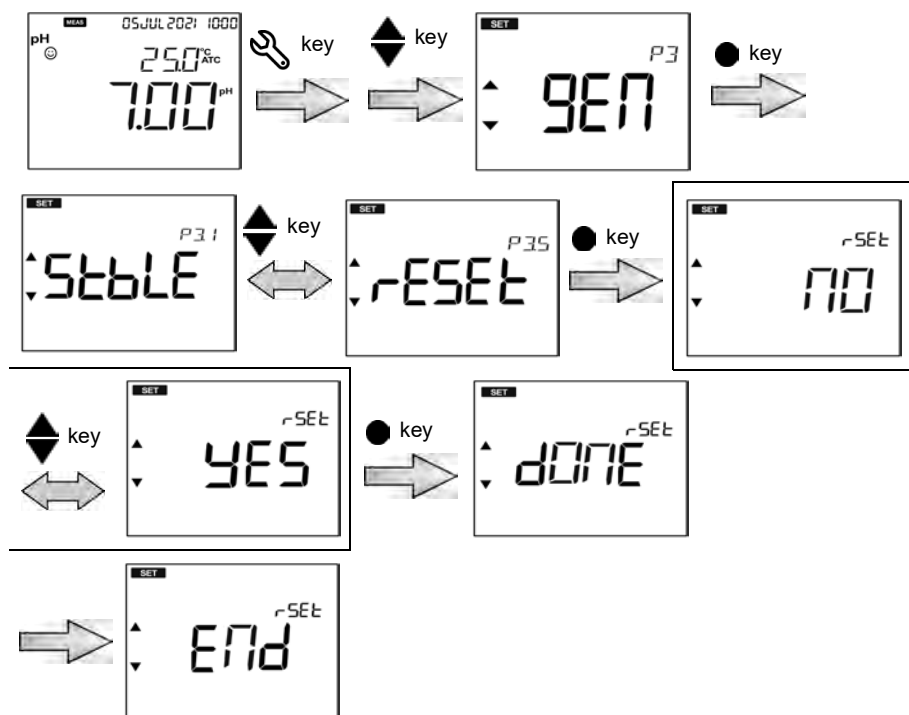

• Clock Setup

Using real-time clock setup, you can set date and time. Follow the procedure detailed below:

Prerequisites

- Switch on the meter.
- Keep the meter in either pH or ion or conductivity mode.

Note


- Setting the date and time is necessary before using the instrument for the first time.
 - Date and time are captured correctly when saving measurement data in the internal memory.
-

Tip

To return to the measurement mode, press the  key.


• Date Setup

1. Press the  key, **P1 PH / ION / COND** screen appears.
2. Press the  key, **P2 / P4 DATA** screen appears.
3. Press the  key, **P3 / P5 GEN** screen appears.
4. Press the  key, **P4 / P6 RTC** screen appears.
5. Press the **ENT**  key, **P4.1 / P6.1 DATE** screen appears.
6. Press the **ENT**  key, default set year appears.
7. Use the   and   keys to change the year.
8. Press the **ENT**  key, default set month appears.
9. Use the   keys to change the month.
10. Press the **ENT**  key, default set day appears.
11. Use the   and   keys to change the day.
12. Press the **ENT**  key, **P4.1 / P6.1 DATE** screen appears. This indicates completion of the date setup.

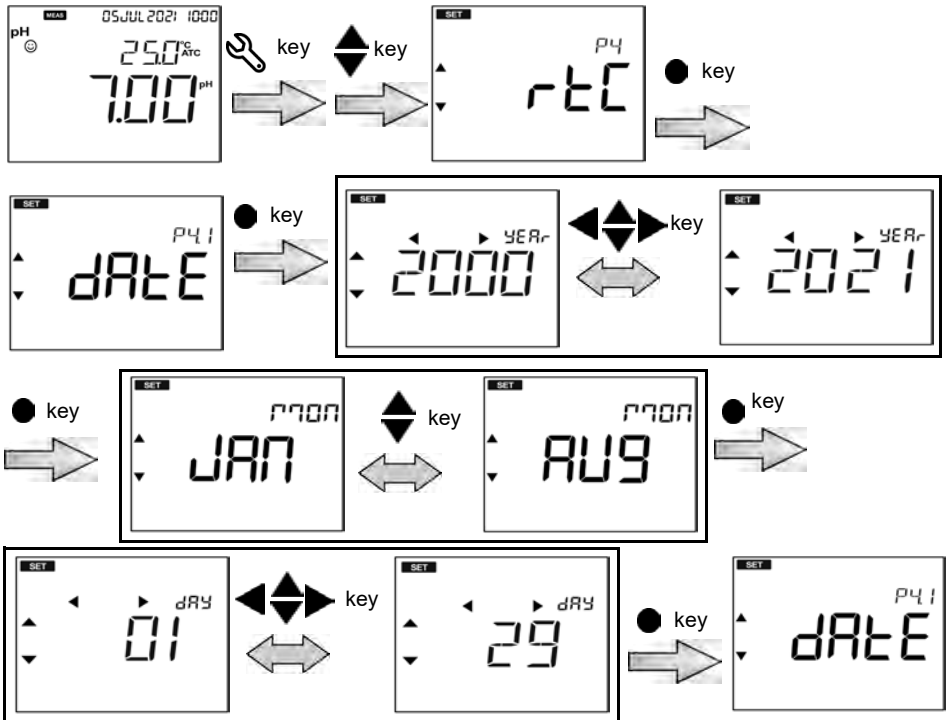

• Time Setup

1. Press the  key, **P1 PH / ION / COND** screen appears.
2. Press the  key, **P2 / P4 DATA** screen appears.
3. Press the  key, **P3 / P5 GEN** screen appears.
4. Press the  key, **P4 / P6 RTC** screen appears.
5. Press the **ENT**  key, **P4.1 / P6.1 DATE** screen appears.
6. Press the  key, **P4.2 / P6.2 TIME** screen appears.
7. Press the **ENT**  key, default set hour appears.
8. Use the   and   keys to change the hour.
9. Press **ENT**  key, default set minute appears.
10. Use the   and   keys to change the minute.
11. Press **ENT**  key, **P4.2 / P6.2 TIME** screen appears. This indicates completion of the time setup.

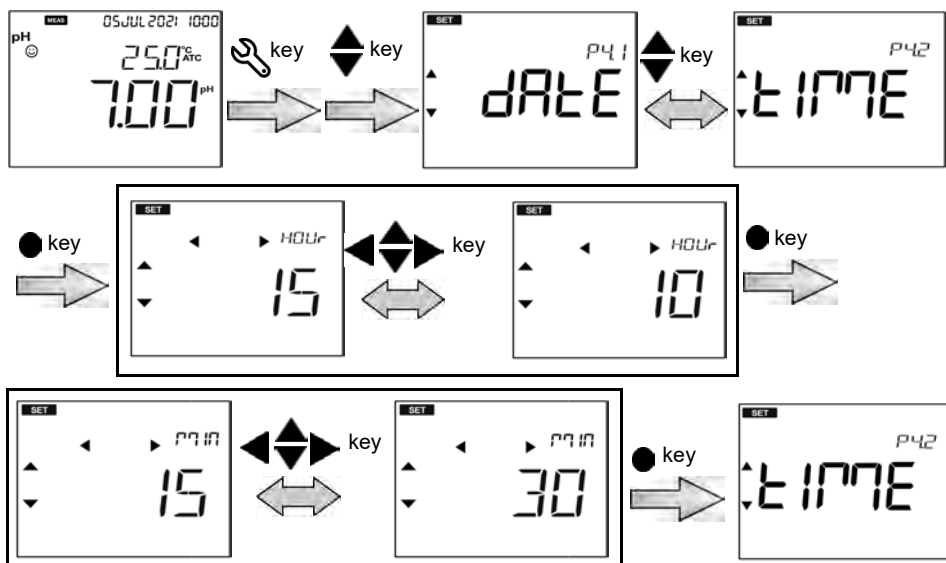

■ Maintenance and Storage

This section describes maintenance and storage of the instrument and the electrodes that are used with the instrument. To use them for a long period, perform the described maintenance procedures appropriately.

● Contact for Maintenance

Please contact your dealer for the product maintenance.

● Maintenance and Storage of the Instrument

- If the instrument is dirty, wipe it gently with a soft dry cloth. If it is difficult to remove the dirt, wipe it gently with a cloth moistened with alcohol.
- The instrument is made of solvent resistant materials but is not resistant to all chemicals. Do not dip the instrument in strong acid or alkali solution, or wipe it with such solutions.
- Do not wipe the instrument with polishing powder or other abrasive compound.

● Environmental Conditions for Storage

- Temperature: 0°C to 45°C
- Humidity: under 80% relative humidity and free from condensation

Avoid the following conditions:

- Dusty place
- Strong vibration
- Direct sunlight
- Corrosive gas environment
- Close to an air-conditioner
- Direct wind

● **Maintenance and Storage of Electrodes**

This section describes an overview of the procedures for maintenance and storage of pH, ORP, ion and conductivity electrodes. For the detailed procedures, refer to the instruction manual for each electrode.

● **How to clean the electrodes**

When the tip of an electrode (responsive membrane and liquid junction) becomes dirty, the response time may slow or an error may occur in the measurement results. To avoid such errors, clean the electrode. For dirt that cannot be washed off by pure water (or deionized water), use the cleaning solution indicated below depending on the type of dirt. After cleaning, rinse the electrode with pure water (or deionized water).

However for pH and ORP electrodes, different cleaning solutions should be used to clean different types of dirt.

For pH Electrode

Type of dirt	Cleaning solution
General	Diluted neutral cleaning solution
Oil	Alcohol, or diluted neutral cleaning solution
Inorganic substance	1 mol/L HCl or electrode cleaning solution
Protein	Cleaning solution including protein-removing enzyme
Alkaline	Dip in 1 mol/L HCl or electrode cleaning solution for 1 h to 2 h

For ORP Electrode

Type of dirt	Cleaning solution
General	Dilute neutral cleaning solution (General dishwashing liquid works reasonably well.)
Oil	
Inorganic substance	Immerse dilute nitric acid (1:1 nitric acid)

• Daily storage of pH and ORP electrodes

If the electrode becomes dry, the response will be slow. Store in a moist atmosphere. Follow the steps below to properly store the electrode:

1. Wash the electrode well with pure water (or deionized water) to remove sample completely, and close the internal solution filler port.
2. Wash the inside of the protective cap with pure water (or deionized water), then add enough pure water (or deionized water) to soak the sponge.
3. Attach the protective cap.

Note

- When the electrode will not be used for a long period, store it by following the electrode storage procedure detailed above.
- For long-term storage of pH and ORP electrodes, replace the reference electrode internal solution with new solution once every 3 to 6 months.

• Daily storage of Ion Electrodes

For the detailed procedures for maintaining and storing electrodes, refer to the instruction manual for each electrode. While the electrode is stored, the concentration of the reference internal solution (outer tube) may change. For this reason, replace the reference internal solution (outer tube) with a dropper or similar tool about once a week to once a month. For conditioning the ion electrodes, refer to the table below:

Ion	Conditioning Solution
Ammonia (NH_3)	Soak the electrode (with membrane cap attached) in a beaker containing filling solution for at least 15 minutes.
Calcium (Ca^{2+})	Soak in 100mg/L (or higher) standard with or without ISA for at least 1 hr.
Chloride (Cl^-)	Soak in 100mg/L (or higher) standard with or without ISA for at least 1 hr.
Fluoride (F^-)	Soak the electrode in 100mg/L or higher without TISAB for at least 1 hr.
Nitrate (NO_3^-)	Soak in 100mg/L (or higher) standard with or without ISA for at least 1 hr.
Potassium (K^+)	Soak in 100mg/L (or higher) standard with or without ISA for at least 1 hr.

Note

For long-term storage of ion electrode, remove the electrode tip and put the rubber cap. Put the protective cap on the electrode. Be sure to keep the protective cap dry. Store both the electrode tip and the electrode in a dry place. Before reuse, condition the electrode.

● **Cleaning the Conductivity Electrode**

Always clean the electrode with deionized water after every measurement. When the response is slow or residue from the sample adheres to the electrode, use the appropriate method below to clean the electrode, and then clean again with deionized water.

Type of dirt	Cleaning solution
General	Diluted neutral cleaning solution
Inorganic substance	Ethanol (keep the ethanol away from plastic parts)
Scale that formed during long term storage	A commercially available scale remover (neutral cleansing solution for kitchen use, etc.) diluted by a factor of 100. If this does not remove the scale, use diluted solution that contains oxygen bleach (sodium percarbonate) or chlorine bleach (sodium hypochlorite).

● **Conductivity Electrode Storage**

If the electrode is stored in a dry state, the cell constant will change. Store with the black electrode part immersed in deionized water, or with the protective cap filled with deionized water and attached to the electrode.

To store the electrode for a long period, clean it well and attach the protective cap filled with deionized water.

■ Error Messages and Troubleshooting

● Error Messages

This section describes the causes of typical errors and the actions to be taken to resolve respective errors. Check these before contacting us.

If ERR is displayed while you are using the instrument, refer to the table below:

Error	Definition	Cause and Solution
OFFS ERR	Offset voltage error	Electrode is dirty or reference junction is clogged. Clean the electrode.
SLPE ERR	Slope error	Electrode sensitivity is low. Please clean and recalibrate with fresh standard solution. If the problem persists, replace the electrode with new one.
BUFF ERR	Cannot auto recognize pH buffer	The instrument cannot identify the pH buffer. Check the calibration solution and use fresh one if required.
STD ERR	Cannot auto recognize standard solution	The instrument cannot identify the standard solution. Check the calibration solution and use fresh one if required.
DATA FULL	Memory data full	The maximum number of saved data has been exceeded. Print or transfer all data then perform data log clear.
	Invalid Operation	Invalid button operation or the input value is out of range. Check the procedure in this manual before operating.
CAL DUE (Electrode icon blinks in MEAS mode)	Calibration past due	Calibration was not performed at the designated interval - the set number of days in calibration alarm setup has passed. Perform calibration.
NOT STBLE	Not stable	ENT  key is pressed before the smiley icon and calibration value have stabilized. Wait for smiley icon and calibration value to stabilize before pressing ENT  key.

Error Messages and Troubleshooting

Error	Definition	Cause and Solution
HIGH OFFS	High offset	Appears when input temperature is below/ above 10°C from original value during temperature calibration.
UNDR RANGE	Under range	Entered value is outside the setting range. Please confirm the setting range and enter value correctly.
OVER RANGE	Over range	
CAL LMT	Calibration limit exceeded	The maximum number of calibration points that can be calibrated has been exceeded. Clear the calibration data.

● Troubleshooting

This section describes causes and actions to take for problems that customers frequently ask.

The indicated value fluctuates

< Problem with the electrode >

Cause	How to solve problem
The electrode is dirty.	Clean the electrode.
The electrode is cracked.	Replace the electrode.
The wrong internal solution is being used.	Use the correct internal solution.
There are air bubbles on the electrode.	Shake the electrode to remove the air bubbles.
The level of internal solution in reference electrode is low.	Replenish the internal solution of the reference electrode until it is higher than the level of the sample.

< Problem with the instrument >

Cause	How to solve problem
There is a motor or other device causing electrical interference.	Measure at a place where no influence from induction is given. Ground all AC-powered equipment.
The electrode is not connected correctly.	Connect the electrode properly.

< Problem with the sample >

Cause	How to solve problem
Electrode is not immersed enough to cover liquid junction.	The electrode must be immersed up to the liquid junction. As a guide, immerse to at least 3 cm from the tip of the electrode.
The stability of electrode is affected by the sample solution.	It is important to select an electrode that is appropriate for the sample. Consult your dealer. To confirm an electrode that is appropriate for the sample, check the pH electrode selection guide in our catalogue, or refer to our website.

The response is slow

Cause	How to solve problem
The electrode is dirty.	Clean the electrode.
The electrode is broken.	Replace the electrode.
The response of electrode is affected by the sample solution.	It is important to select an electrode that is appropriate for the sample. Consult your dealer. To confirm an electrode that is appropriate for the sample, check the pH electrode selection guide in our catalogue, or refer to our website.

The indicated value does not change

Cause	How to solve problem
The electrode is cracked.	Replace the electrode.
The electrode is not connected correctly.	Connect the electrode correctly.
The instrument is in HOLD state.	Cancel the HOLD state.
Instrument defect.	Consult your dealer.

The measured value is out of the measurement range

When the measured value is below the display range, "Ur" appears. When the measured value is over the display range, "Or" appears.

Cause	How to solve problem
Sample is out of the measurement range.	Use a sample within the measurement range.

Error Messages and Troubleshooting

Cause	How to solve problem
Electrode is not immersed enough to cover liquid junction.	The electrode must be immersed up to the liquid junction. As a guide, immerse to at least 3 cm from the tip of the electrode.
The electrode cable is broken.	Replace the electrode.
Calibration is not performed or performed incorrectly.	Perform calibration correctly.
Instrument defect.	Check as explained below.

• How to check for instrument defect

Short the metal part of the outer tube to the center pin of the electrode connector of the corresponding channel of the instrument. If the measured value blinks or does not show zero, consult your dealer.



Repeatability of the measured value is poor

Cause	How to solve problem
Effect of the sample solution.	Repeatability becomes poor when the pH of the sample changes over time.
The electrode is dirty.	Clean the electrode.
The electrode is broken.	Replace the electrode.
The internal solution of the electrode runs out or contaminated.	Replace the internal solution with new one.
The level of internal solution in reference electrode is low.	Replenish the internal solution of the reference electrode until it is higher than the level of the sample.

Nothing appears when the power is turned ON

Cause	How to solve problem
Instrument defect.	Consult your dealer.
Power is not supplied.	Connect the AC adapter.

Swelling of keypad

Cause	How to solve problem
Using the instrument at high elevation or other location where the air pressure is different from sea level.	To eliminate the pressure difference between the inside and outside of the instrument, briefly open and then close the serial connector cover. After opening, correctly close the cover to maintain dust and water proofing.
Instrument defect.	Consult your dealer.

Part of the display is missing

Cause	How to solve problem
Instrument defect.	Check the display by switching ON the instrument when all the LCD segments are lit.

■ Appendix

This section describes the technical information, printer formats, and specifications of the instrument.

● Appendix 1

pH calibration can be performed according to several buffer standards. The most common standard is the US buffer standard. The default setup is US buffer standard. Alternative standards that can be chosen are NIST, NIST2, DIN and CUST (Custom).

The pH buffers are temperature dependent i.e. the pH value changes with change in temperature. The meter is intelligent to detect the temperature and pH value associated with buffer when calibration is performed. It remembers all the temperature vs. pH value for all the standards.

The pH vs. temperature values for the various standards are listed below:

< USA >

Temp. (°C)	pH 1.68	pH 4.01	pH 7.00	pH 10.01	pH 12.46
0	1.67	4.01	7.12	10.32	13.42
5	1.67	4.01	7.09	10.25	13.21
10	1.67	4.00	7.06	10.18	13.00
15	1.67	4.00	7.04	10.12	12.81
20	1.68	4.00	7.02	10.06	12.63
25	1.68	4.01	7.00	10.01	12.45
30	1.69	4.01	6.99	9.97	12.29
35	1.69	4.02	6.98	9.93	12.13
40	1.70	4.03	6.97	9.89	11.98
45	1.70	4.04	6.97	9.86	11.84
50	1.71	4.06	6.97	9.83	11.70
55	1.72	4.08	6.97	9.81	11.57

< NIST >

Temp. (°C)	pH 1.68	pH 4.01	pH 6.86	pH 9.18	pH 12.46
0	1.67	4.01	6.98	9.46	13.42
5	1.67	4.01	6.95	9.39	13.21
10	1.67	4.00	6.92	9.33	13.00
15	1.67	4.00	6.90	9.27	12.81
20	1.68	4.00	6.88	9.22	12.63
25	1.68	4.01	6.86	9.18	12.45
30	1.69	4.01	6.85	9.14	12.29
35	1.69	4.02	6.84	9.10	12.13
40	1.70	4.03	6.84	9.07	11.98
45	1.70	4.04	6.83	9.04	11.84
50	1.71	4.06	6.83	9.01	11.70
55	1.72	4.08	6.83	8.99	11.57

< NIST2 >

Temp. (°C)	pH 1.68	pH 4.01	pH 6.86	pH 10.01	pH 12.46
0	1.67	4.01	6.98	10.32	13.42
5	1.67	4.01	6.95	10.25	13.21
10	1.67	4.00	6.92	10.18	13.00
15	1.67	4.00	6.90	10.12	12.81
20	1.68	4.00	6.88	10.06	12.63
25	1.68	4.01	6.86	10.01	12.45
30	1.69	4.01	6.85	9.97	12.29
35	1.69	4.02	6.84	9.93	12.13
40	1.70	4.03	6.84	9.89	11.98
45	1.70	4.04	6.83	9.86	11.84
50	1.71	4.06	6.83	9.83	11.70
55	1.72	4.08	6.83	9.81	11.57

< DIN >

Temp. (°C)	pH 1.09	pH 3.06	pH 4.65	pH 6.79	pH 9.23	pH 12.75
0	1.08	3.10	4.67	6.89	9.48	13.37
5	1.09	3.10	4.66	6.87	9.43	13.37
10	1.09	3.10	4.66	6.84	9.37	13.37
15	1.09	3.08	4.65	6.82	9.32	13.17
20	1.09	3.07	4.65	6.80	9.27	12.96
25	1.09	3.06	4.65	6.79	9.23	12.75
30	1.10	3.05	4.65	6.78	9.18	12.61
35	1.10	3.04	4.65	6.77	9.13	12.45
40	1.10	3.04	4.66	6.76	9.09	12.29
45	1.11	3.04	4.67	6.76	9.04	12.14
50	1.11	3.04	4.68	6.76	9.00	11.98
55	1.11	3.04	4.69	6.76	8.96	11.84

Note

Calibration is performed using Nernst's equation with the above values.

Conductivity Standard Values at Various Temperatures

Temp. (°C)	Conductivity value at 25°C			
	84 (µS/cm)	1413 (µS/cm)	12.88 (S/cm)	111.8 (mS/cm)
15	68	1147	10.48	92.5
16	70	1173	10.72	94.4
17	71	1199	10.95	96.3
18	73	1225	11.19	98.2
19	74	1251	11.43	100.2
20	76	1278	11.67	102.1
21	78	1305	11.91	104.0
22	79	1332	12.15	105.9
23	81	1359	12.39	107.9
24	82	1386	12.64	109.8
25	84	1413	12.88	111.8
26	86	1440	13.13	113.8
27	87	1467	13.37	115.7
28	89	1494	13.62	117.7
29	90	1521	13.87	119.7
30	92	1548	14.12	121.8
31	94	1575	14.37	123.9

● **Appendix 2**

Printer Format - Measurement

pH

Model	PC2000
S/No	A81J1234
SW Rev	1.00
Date	23APR2021
Time	09:41:48
Mode	pH
Stability	STABLE
pH	4.21 pH
mV	151.4 mV
Temp.	23.7 C (ATC)
Electrode	EXCELLENT
User Name	
Signature	

mV

Model	PC2000
S/No	A81J1234
SW Rev	1.00
Date	23APR2021
Time	09:41:48
Mode	mV
Stability	STABLE
mV	151.4 mV
Temp.	23.7 C (ATC)
User Name	
Signature	

Relative mV

Model	PC2000
S/No	A81J1234
SW Rev	1.00
Date	23APR2021
Time	09:41:48
Mode	R.mV
Stability	STABLE
R.mV	147.8 R.mV
Offset	-3.4 mV
Temp.	24.1 C (ATC)
User Name	
Signature	

Ion

Model	PC2000
S/No	A81J1234
SW Rev	1.00
Date	23APR2021
Time	12:20:37
Mode	ION
Stability	STABLE
ION	0.102 g/L
mV	-17.6 mV
Temp.	25.0 C (MAN)
Electrode	EXCELLENT
User Name	
Signature	

Conductivity

Model	PC2000
S/No	A81J1234
SW Rev	1.00
Date	23APR2021
Time	14:02:15
Mode	CONDUCTIVITY
Stability	STABLE
Cond	1420 μ S/cm
Temp.	23.3 C (ATC)
CellConst.	1.052
Temp.Coeff	2.00
Ref. Temp	25.0 Deg C
Electrode	EXCELLENT
User Name	
Signature	

Resistivity

Model	PC2000
S/No	A81J1234
SW Rev	1.00
Date	23APR2021
Time	14:33:21
Mode	RESISTIVITY
Stability	STABLE
Resist	722.9 Ohm-cm
Temp.	22.4 C (ATC)
CellConst.	1.052
Temp.Coeff	2.00
Ref. Temp	25.0 Deg C
User Name	
Signature	

Salinity

Model	PC2000
S/No	A81J1234
SW Rev	1.00
Date	23APR2021
Time	14:15:16
Mode	SALINITY
Stability	STABLE
Salinity	0.7 ppt
Temp.	22.9 C (ATC)
CellConst.	1.052
Temp.Coeff	2.00
Ref. Temp	25.0 Deg C
Electrode	EXCELLENT
User Name	
Signature	

TDS

Model	PC2000
S/No	A81J1234
SW Rev	1.00
Date	23APR2021
Time	14:09:42
Mode	TDS
Stability	STABLE
TDS	711 mg/L
Temp.	23.0 C (ATC)
CellConst.	1.052
Temp.Coeff	2.00
Ref. Temp	25.0 Deg C
Electrode	EXCELLENT
User Name	
Signature	

Printer Format - Data Log

Model	PC2000
S/No	A81J1234
SW Rev	1.00
User Name	
Signature	
Logged Data	
Location	18
Date	23APR2021
Time	14:33:04
Mode	RESISTIVITY
Stability	STABLE
Resist	722.9 Ohm-cm
Temp.	22.4 C (ATC)
CellConst.	1.052
Temp.Coeff	2.00
Ref.Temp	25.0 Deg C
Location	17
Date	23APR2021
Time	14:15:04
Mode	SALINITY
Stability	STABLE
Salinity	0.7 ppt
Temp.	22.9 C (ATC)
CellConst.	1.052
Temp.Coeff	2.00
Ref.Temp	25.0 Deg C
Electrode	EXCELLENT
Location	16
Date	23APR2021
Time	14:09:49
Mode	TDS
Stability	STABLE
TDS	711 mg/L
Temp.	23.0 C (ATC)
CellConst.	1.052
Temp.Coeff	2.00
Ref.Temp	25.0 Deg C
Electrode	EXCELLENT
Location	15
Date	23APR2021
Time	14:02:04
Mode	CONDUCTIVITY
Stability	STABLE
Conductivity	1419 µS/cm
Temp.	23.5 C (ATC)
CellConst.	1.052
Temp.Coeff	2.00
Ref.Temp	25.0 Deg C
Electrode	EXCELLENT
Location	14
Date	23APR2021
Time	12:23:39
Mode	ION
Stability	Stable
ION	0.102 µ/L
mV	117.6 mV
Temp.	25.0 C (MAN)
Electrode	EXCELLENT
Location	13
Date	23APR2021
Time	11:28:13
Mode	pH
Stability	STABLE
pH	4.03 pH
mV	162.3 mV
Temp.	23.8 C (ATC)
Electrode	EXCELLENT
Location	12
Date	23APR2021
Time	10:38:24
Mode	R.mV
Stability	STABLE
R.mV	750.3 R.mV
Offset	-3.4 mV
Temp.	23.8 C (ATC)
Location	11
Date	22APR2021
Time	10:00:46
Mode	mV
Stability	STABLE
mV	212.3 mV
Temp.	25.0 C (MAN)

Printer Format - Calibration

pH

Model		PC2000
S/No		A81J1234
SW Rev		1.00
Date		23APR2021
Time		09:41:48
Calibration Data		
Cal Date		08APR2021
Cal Time		12:29:58
Cal Points:		
pH	mV	Slope
4.01	163.2	98.9%
7.00	-11.3	
10.01	-185.7	98.1%
Offset		-11.0 mV
Avg Slope		98.5%
Temp.		23.3 C (ATC)
Electrode		EXCELLENT
User Name		
Signature		

Ion

Model	PC2000	
S/No	A81J1234	
SW Rev	1.00	
Date	23APR2021	
Time	12:25:49	
Calibration Data		
Cal Date	09APR2021	
Cal Time	17:32:01	
Cal Points:		
Ion Value	mV	Slope
0.100 g/L	-17.2	98.4%
1.000 g/L	-75.4	
Avg Slope		98.4%
Cal. Temp.	25.0 C (MAN)	
Electrode	EXCELLENT	
User Name		
Signature		

Conductivity

Model	PC2000
S/No	A81J1234
SW Rev	1.00
Date	23APR2021
Time	13:53:51
Calibration Data	
Cal Date	23APR2021
Cal Time	13:51:23
Cal Points:	
Value	Cal Factor
84.0 $\mu\text{S}/\text{cm}$	1.003
1413 $\mu\text{S}/\text{cm}$	1.039
12.88 mS/cm	1.051
111.8 mS/cm	1.068
Avg. CalFac	1.040
Temp.	23.7 C (ATC)
Electrode	EXCELLENT
User Name	
Signature	

Salinity

Model	PC2000
S/No	A81J1234
SW Rev	1.00
Date	23APR2021
Time	13:39:47
Calibration Data	
Cal Date	09APR2021
Cal Time	15:30:43
Cal Point	70.0 ppt
Avg. CalFac	1.006
Temp.	23.2 C (ATC)
Electrode	EXCELLENT
User Name	
Signature	

● **Meter Specifications**

Specifications	Environmental Express Series 2000
pH Range	-2.000 to 20.000 pH
Resolution	0.1 / 0.01 / 0.001 pH
Accuracy	± 0.003 pH
pH Buffer Groups	USA, NIST, NIST2, DIN, Custom
Calibration Points	Up to 5 (USA, NIST, NIST2) / Up to 6 (DIN, Custom)
ORP Range	± 2000.0 mV
Resolution	0.1 mV
Accuracy	±0.2 mV
Calibration Option	Yes (Up to ±200 mV)
Ion Range	0.000 µg/L to 9999 g/L
Units	µg/L ↔ mg/L ↔ g/L, ppm ↔ ppt, mmol/L ↔ mol/L
Resolution	4 Significant digits
Accuracy	± 0.3% full scale or ± 0.2 mV, whichever is higher
Calibration Points	Up to 5
Conductivity Range	0.000 to 1.999 µS/cm (k = 0.1) 2.00 to 19.99 µS/cm (k = 0.1, 1) 20.0 to 199.9 µS/cm (k = 0.1, 1, 10) 200 to 1999 µS/cm (k = 0.1, 1, 10) 2.00 to 19.99 mS/cm (k = 0.1, 1, 10) 20.0 to 199.9 mS/cm (k = 1, 10) 0.200 to 2.000 S/cm (k = 10)
Units	Auto ranging S/cm, S/m (µS ↔ mS)
Resolution	0.05% full scale
Accuracy	± 0.6% full scale, ± 1.5% full scale > 18.0 mS/cm
Reference Temperature	15.0 to 30.0 °C (adjustable)
Temperature Coefficient	0.00 to 10.00% per °C (adjustable)
Cell Constants	0.0700 to 13.000 (adjustable)
Calibration Points	Up to 4 (Auto) / Up to 5 (Manual)

Specifications	Environmental Express Series 2000
Resistivity Range	0.000 $\Omega\cdot\text{cm}$ to 20.0 $\text{M}\Omega\cdot\text{cm}$
Resolution	0.5% full scale
Accuracy	$\pm 0.6\%$ full scale; $\pm 1.5\%$ full scale > 1.80 $\text{M}\Omega\cdot\text{cm}$
Total Dissolved Solids (TDS) Range	0.01 to 9.99 mg/L (ppm) 10.0 to 99.9 mg/L (ppm) 100 to 999 mg/L (ppm) 1.00 to 9.99 g/L (ppt) 10.0 to 100 g/L (ppt)
Resolution	0.01, 0.1, 1 mg/L $\leftrightarrow$ g/L (ppm $\leftrightarrow$ ppt)
Accuracy	$\pm 0.1\%$ full scale
TDS Curves	EN27888, 442, NaCl, Linear (0.40 to 1.00)
Salinity Range	0.0 to 100.0 ppt / 0.00 to 10.00 %
Resolution	0.1 ppt / 0.01%
Accuracy	$\pm 0.2\%$ full scale
Salinity Curves	NaCl / Seawater
Calibration Option	Yes
Temperature Range	-30.0 to 130.0 $^{\circ}\text{C}$ / -22.0 to 266.0 $^{\circ}\text{F}$
Resolution	0.1 $^{\circ}\text{C}$ / $^{\circ}\text{F}$
Accuracy	± 0.5 $^{\circ}\text{C}$ / ± 0.9 $^{\circ}\text{F}$
Calibration Option	Yes (± 10.0 $^{\circ}\text{C}$ / ± 18.0 $^{\circ}\text{F}$ range in 0.1 $^{\circ}\text{C}$ increment)
Memory	2000 data sets
Auto Data Log	Yes
Real-time Clock	Yes
Date & Time Stamp	Yes
Measurement Modes	Auto Stable / Auto Hold / Real Time
Offset & Slope Display	Yes (Segment & Average Slopes)
Calibration Alarm	Yes (Programmable: up to 90 days)
Auto Shut-Off	Yes (Programmable: up to 30 mins.)
Electrode Status	On screen display
Diagnostics	Yes

Meter Specifications

Specifications	Environmental Express Series 2000
Password Setting	Yes
Software Upgrade	Yes
PC / Printer Communication	Phono jack (USB / RS232)
Meter Inputs	BNC, phono (ATC), DC sockets
Display	5" Custom LCD with 320 segments and backlight
Power Rating AC Adapter	Input Voltage: 100 – 240VAC +/- 10%, 50/60Hz
Power Rating Instrument	Input Voltage: 7V
	Power Consumption: 0.7 W / 100 mA
Dimensions	155 (L) x 150 (W) x 67 (H) mm
Weight	Approx 765g for PH2000 benchtop meter
	Approx 765g for ION2000 benchtop meter
	Approx 765g for EC2000 benchtop meter
	Approx 770g for PC2000 benchtop meter
Electrode Stand	Integrated
Warranty	3 years

• Table of Conductivity Cell Range

• Unit: S/m

Display Range	Cell Constant		
	0.1 cm^{-1}	1 cm^{-1}	10 cm^{-1}
OR (Over Range)	1 S/m ~ 0.01 mS/m	10 S/m ~ 0.1 mS/m	100 S/m ~ 1 mS/m
20.0 ~ 200.0 S/m			
2.00 ~ 20.00 S/m			
0.200 ~ 1.999 S/m			
20.0 ~ 199.9 mS/m			
2.00 ~ 19.99 mS/m			
0.000 ~ 1.999 mS/m			

• Unit: S/cm

Display Range	Cell Constant		
	0.1 cm^{-1}	1 cm^{-1}	10 cm^{-1}
OR (Over Range)	10 mS/cm ~ 0.1 μ S/cm	100 mS/cm ~ 1 μ S/cm	1000 mS/cm ~ 10 μ S/cm
0.200 ~ 2.000 S/cm			
20.0 ~ 199.9 mS/cm			
2.00 ~ 19.99 mS/cm			
200 ~ 1999 μ S/cm			
20.0 ~ 199.9 μ S/cm			
2.00 ~ 19.99 μ S/cm			
0.000 to 1.999 μ S/cm			

• Table of Conductivity Cell Range (Resistivity Range)

• Unit: $\Omega \cdot \text{cm}$

Display Range	Cell Constant		
	0.1 cm^{-1}	1 cm^{-1}	10 cm^{-1}
OR (Over Range)	10 $\text{M}\Omega \cdot \text{cm}$ ~ 100 $\Omega \cdot \text{cm}$	1 $\text{M}\Omega \cdot \text{cm}$ ~ 10 $\Omega \cdot \text{cm}$	100 $\text{K}\Omega \cdot \text{cm}$ ~ 1 $\Omega \cdot \text{cm}$
1.0 ~ 20.0 $\text{M}\Omega \cdot \text{cm}$			
0.001 ~ 0.999 $\text{M}\Omega \cdot \text{cm}$			
(0.0 ~ 999.9 $\Omega \cdot \text{cm}$)			



USA Tel: 800-343-5319 Intl. Tel: +1 843-881-6560
Email: info@envexp.com Website: www.environmentalexpress.com

For any questions regarding this product, please contact your local agency.

Local: M004290
P/N: 3200928091
GZ: 0000657564