



Welcome

KANE458s

Flue Gas Analyser with
direct CO, CO₂ & CO
sensor protection

Quick reference guide



Hello KANE458s getting started

- 1 Know your KANE458s
- 2 Connections
- 3 Before use
- 4 KANE ASSET MANAGEMENT (KAM)

Please register your analyser at www.kane.co.uk & download the full instruction manual from our product selector

PLEASE READ ALL SAFETY WARNINGS IN THE MANUAL

1

Know your KANE458s




Function keys

Icon	Description
	Data hold - Short press to hold current data on screen
	Pump toggle - Long press to toggle pump on & off
	Navigate Up - Short press to scroll up
	Enter key - Used to select current option
	Navigate Down - Short press to scroll down
	Save log - Long press to store data
	Print report - Short press to print a report

2

Connections

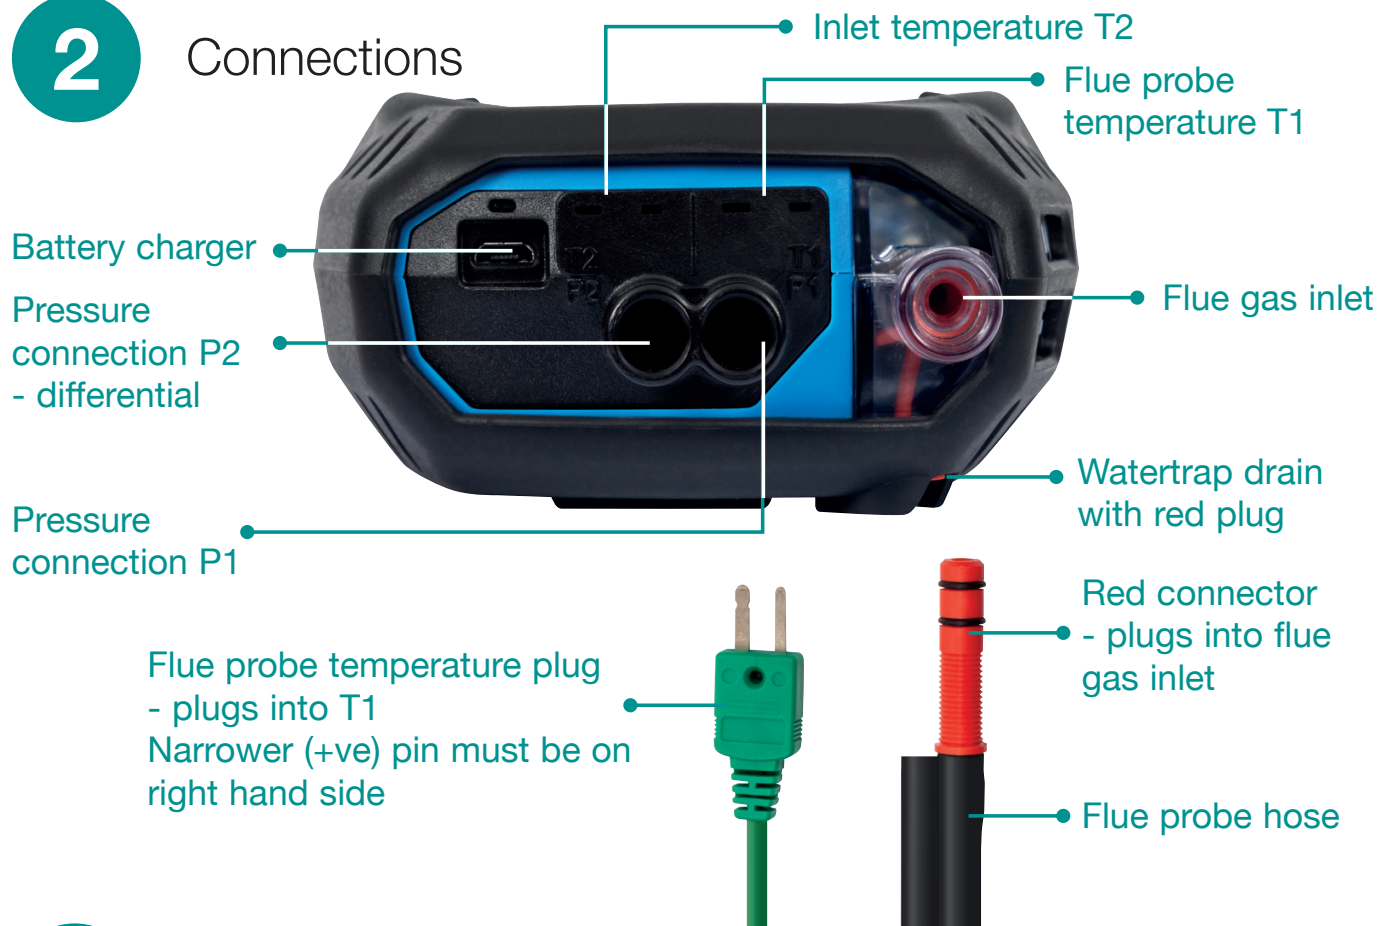

3

Before use

Check

Particle filter is not dirty; Water trap & flue probe empty of water;
 Water trap & red plug fitted to analyser; Flue probe hose connected to flue gas inlet;
 Flue probe temperature plug connected to T1 temperature connection

Fresh air purge


Position flue probe in fresh air & press "On/Off"
 Analyser auto-calibrates within 60 seconds
 Select "Ratio" on dial - in fresh air CO reading = 0ppm
 Select "O₂/Eff" on dial - in fresh air O₂ reading = 20.9%
 Select "Status" on dial to view

For best pressure sensor accuracy

Switch analyser on for 5 minutes to let temperature stabilise
 Zero pressure sensor when analyser in exact position of use

To charge NiMH rechargeable batteries

Switch off
 Connect charger - charging indicator illuminates
 Display shows "BATTERY CHARGING" if batteries need charging



Sensor upgrades
available

4

KANE ASSET MANAGER (KAM)



Register your KANE analyser to create your KAM dashboard:

- ★ Simple online booking
- ★ Relevant product specific promotions, special offers & discounts
- ★ Automatic reminder when due for recertification
- ★ **FREE POSTAGE** returning your KANE analyser
- ★ **SAME DAY** annual FGA recertification **OR YOUR MONEY BACK***

*Excludes KANE '9 series' analysers & UKAS certificates

Use all 11 digits

182620200
92



PLEASE READ ALL SAFETY WARNINGS IN THE MANUAL

Follow us on...



★ Trustpilot



KANE and the KANE logo (registered in the UK and elsewhere) are trademarks of Kane Group Limited, used under licence.
All other marks are trademarks of their respective holders. © 2020 Kane International Limited

Stock No. QRG00088 Rev: 1.20720